

Fischer Accessories



H·G·Fischer & Company, Inc.
Physical Therapy Headquarters
2323-37 Wabansia Avenue
Chicago, Illinois

FISCHER

PHYSICAL THERAPY SUPPLIES *and* ACCESSORIES

Catalog No. 22
January, 1929



H. G. FISCHER & COMPANY, Inc.
Physical Therapy Headquarters
2323-37 Wabansia Avenue
Chicago, Illinois

Foreword

IN presenting this, the 22nd edition of our Accessory Catalog, we wish to call special attention to the many additions and changes that have been made. This catalog supersedes all former issues. It shows our full line of accessories, and renders obsolete all former illustrations, prices and description.

We believe that our successful growth has been largely due to the rigid policies which we adopted at the outset—up-to-date manufacturing equipment, fair selling prices, guaranteed shipments, an adequate Service Department, and the ever present desire to “play square.”

How to Order Always use a separate sheet on which to write your order, and write it on *one* side only. *Avoid* including it in the wording of your letter. This hastens the correct filling of your order. Use catalog numbers and write plainly, and when ordering by telegraph use *Code* words as they designate to us exactly what is desired, and save you expense in the message as well.

State clearly whether your machine is to be operated on the Direct or Alternating Current. If on D. C., give Voltage; if on Alternating, give Voltage and Cycle. Obtain this information from a reliable source; preferably from your electric power station.

When order does not give shipping instructions we will send via the most direct route. Articles of light weight will be sent by Parcel Post to expedite delivery wherever possible.

Damage to Goods in Transit Our responsibility ceases when goods are receipted for by the express freight carrier, agent or Post Office, and we cannot be held responsible for breakage during transit, and if claim has to be filed for damaged goods, such claim should be filed by the consignee against the Transportation Company.

Return of goods by parcel post should always be insured so the shipper is protected in case parcels are lost.

As soon as it is found that goods are received in a damaged condition the carrier's agent should at once be notified and have the damaged goods inspected.

Neglect in complying with this rule places the responsibility entirely with the consignee in case claim is refused.

Guarantee Any defects in our apparatus that may develop within six (6) months from date of shipment under normal and proper use, due to faulty material, imperfect insulation, or careless workmanship, will be repaired or replaced at our option and our expense, provided such apparatus is delivered *prepaid* to our factory.

For repairs or replacements during the next twelve (12) months, we will charge only actual cost to cover, and after this period our service and our attention are to be called on when required, with the understanding that charges for overhauling "Fischer" apparatus will always remain as near actual cost as possible. We do not maintain a repair department for profit — this department is entirely for your service.

We will not assume any liability for work done by others, without our consent in writing, nor for defects from improper storage.

We will not assume any liability for breakage of glassware, lamps, or X-ray plates, nor for deterioration of rubber goods, X-ray films or any perishable goods. We can but use the best materials obtainable.

Rotary converters, meters, and motors not manufactured by us do not carry our guarantee, but are backed up by the guarantee of the makers.

Return of Merchandise

Crediting for return of goods ordered in error or on account of dissatisfaction on receipt has become a serious factor of expense, and is a problem difficult of solution. In justice to our customers, and to ourselves we have adopted the following, governing such returns:

No merchandise will be returnable for credit after having been in customer's possession fifteen (15) days or more.

No merchandise will be returnable for credit except upon written request of purchaser, and then only with our consent.

All merchandise must be returned *prepaid*.

No merchandise will be accepted unless returned in salable condition.

All merchandise returned, whether for repairs or for credit, must be carefully packed, and all goods over a \$2.00 valuation should be insured.

Cabinets or Portables returned for repairs or overhauling should be stripped of all accessories, unless such accessories are also to be gone over. Loose accessories always mean danger or further damage to your equipment in shipping. We cannot be held responsible for breakage or damages due to improper packing.

And last, but very important nevertheless, *never* fail to place your name and address in and on the box or parcel when shipping to us.

Prices All prices are figured F. O. B. Chicago. The prices quoted in this catalog on all our goods are as low as it is possible to make them and still be consistent with the quality of the materials and high grade of workmanship used in their construction.

All orders for \$1.00 or under should be accompanied with stamps, money order or check.

Our minimum billing for goods shipped is 50c.

Our prices are subject to change without notice.

Terms Retail purchasers having an established credit with us may discount their bills in ten days, or they will be considered net and due in thirty days.

Our goods are also sold on the deferred payment plan. We shall be glad to make quotations to reliable persons, and ask that you write us if interested.

New Accounts

We earnestly solicit new accounts, but purchasers will appreciate the necessity of supplying satisfactory references. The name of the bank carrying your account, or some Chicago firm with which you have transacted former business, is usually sufficient.

NOTICE!

Illustrations herewith are not binding as to details, in view of constant improvements, and the goods supplied you may differ slightly in appearance. However, when your order is received, the very latest model will always be forwarded. Prices quoted are subject to change without notice.


The Fischer Flexible Mesh Electrodes

The most flexible and convenient ALL-METAL electrode ever designed.


Fits any part of the body like a glove, regardless of shape or contour.

Composed of a series of flat links of German silver, they are flexible, practically indestructible, easily sterilized, and form an almost continual flat surface to be applied to the skin.


Especially valuable for use on uneven surfaces where solid electrodes cannot be effectively employed — on the knee, elbow, wrist, hand, spine, over the shoulder, in fact wherever it is impossible to make perfect contact with any other means.

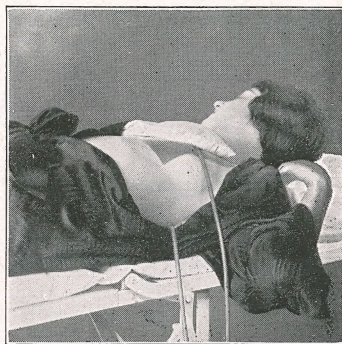

Application Mesh Electrode



A Mesh Electrode



Section of Electrode, Showing Exact Size of Links.

Stocked in the following sizes:

No.		Code	Price
845	4"x 6"	Samar	\$1.20
847	6"x 6"	Samil	1.80
848	6"x 8"	Samme	2.40
846	8"x 8"	Sambo	3.20
849	8"x10"	Samot	4.00
850	10"x12"	Sampa	6.00

Or we can furnish as follows:


No.		Code	Price
843	3" wide	Sabbot	Per inch, \$0.20
844	6" wide	Safrol	30
870	8" wide	Sagger	40
871	10" wide	Sagums	50
872	12" wide	Sailer	60

(Will be cut to any lengths, to order. A cutting charge of 15c will be added for special lengths under 10 inches.)


Can be folded to cover any area.

Cuff Method Diathermy Application

For employing the "Cuff Method" of applying diathermy to the limbs and joints, every physician should have at least one pair of Mesh Electrode Cuffs. These are strips of German Silver Mesh, 3 inches wide and from 12 to 24 inches long, with an arrangement fastened to one end for holding the elastic bandage. Very convenient and handy, and once used will be found indispensable.



No.		Code	Price
900	Mesh Cuff and Clamp—3"x12"	Nephew	\$3.25
901	Mesh Cuff and Clamp—3"x16"	Neptun	4.50
902	Mesh Cuff and Clamp—3"x20"	Nereid	5.00
903	Mesh Cuff and Clamp—3"x24"	Neroli	5.30

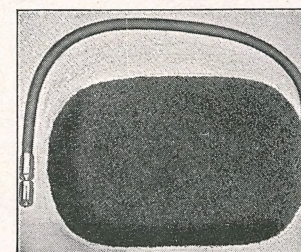

Sponge Pad Electrode

Lay this pad in your tray or pan of salt water, and your patient will not complain of hot spots when placing hand or foot down for contact.


No.	Code	Price
886	Nether	\$2.25

Mesh Electrodes With Sponge Rubber Pads

These combinations are the direct result of numerous suggestions that they would be very adaptable; already they have more than fulfilled expectations.

The Sponge Rubber padding may be washed and always kept clean. It is very soft, and conforms well to any uneven surface. Stocked in three sizes:

No.		Code	Price
891	Sponge Mesh Electrode—3"x3½"	Nemean	\$3.40
893	Sponge Mesh Electrode—4"x4½"	Neogae	4.30
894	Sponge Mesh Electrode—4½"x5"	Neolgy	4.85


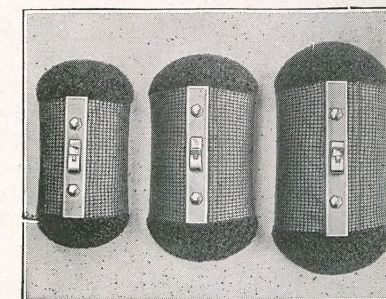


No. 891 No. 893 No. 894

Sponge Rubber Pads

No.		Code	Price
896	Sponge pad, only, 3 x 3½"	Weaner	\$0.40
897	Sponge pad, only, 4 x 4½"	Weapon	.75
898	Sponge pad, only, 4½x5"	Watery	1.10


The Universal Diathermy Clamp Electrode

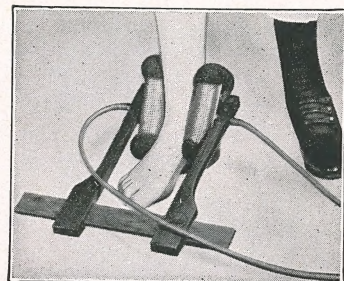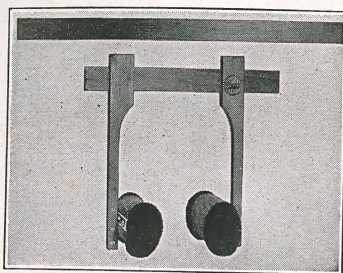

Applied and removed in an instant—may be used on practically any part of the body. All of the various sponge mesh electrodes described on page 7 are interchangeable on this device.

No.		Code	Price
929	Universal Diathermy Clamp, with 3-in. sponges.....	<i>Smacla</i>	\$11.75
930	The Universal Diathermy Clamp Electrode.....	<i>Uclamp</i>	13.00

Metal Connector For Mesh Electrodes




A simple device to fit the No. 1330 Fischer Diathermy Cords. Made of spring brass, heavily nickel-plated. Cord tip cannot come loose when once snapped in place. The contact is flat, but there are several small teeth protruding for engaging the surface of the electrode to prevent slipping. On the limbs this device should be held in place with our No. 854 Elastic Bandage; on the body, with a sandbag.

No.		Code	Price
851	Metal Connector	<i>Mescon</i>	\$0.10

Fischer Multiple Cord Connector

Used when two, three or even four cord connections are desirable from one terminal.




Catalog No. 865

The small end tip is fastened into the proper binding post on your machine, and you may carry as many cords from it as desired.

No.		Code	Price
865	Multiple Connector 5-Wire.....	<i>Sable</i>	\$1.50
866	Multiple Connector 3-Wire.....	<i>Sabin</i>	1.00

Sandbags

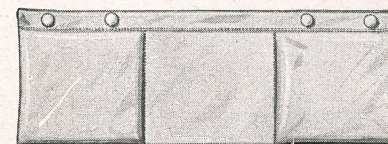


No. 880

Made of tough linen fabric. The end, or sand pockets are of the same size and capacity regardless of the length of the whole, and are about half filled with sand. This leaves the assembly very flexible and adaptable.

When the bag is placed over the patient the flat band only bears on the electrode—the weights hang down at the sides. The longer pads are made to hang over the side of the treatment table or cot.

No.		Code	Price
880	5" wide by 15" long.....	<i>Nestor</i>	\$1.60
881	5" wide by 25" long.....	<i>Sanbag</i>	2.00
882	5" wide by 36" long.....	<i>Neting</i>	2.20
883	5" wide by 45" long.....	<i>Sannes</i>	2.40
884	5" wide by 60" long.....	<i>Neubag</i>	2.50

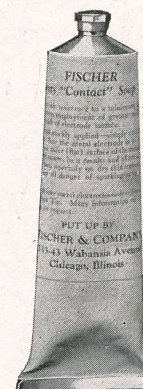


No. 876

Fischer Improved Diathermy Paste



No. 906



No. 907

Convenient, always ready.


No.		Code	Price
876	In handy collapsible 10 oz. tube.....	<i>Diasop</i>	\$0.80
906	16 oz. opalite jar.....	<i>Votive</i>	1.00
907	16 oz. refill for jar, in wax paper carton.....	<i>Vowels</i>	.90

Elastic Bandage


Employing Elastic Bandage is the only known method of binding Diathermy Electrodes to the limbs, which will permit the patient to move if necessary for the sake of comfort without the electrode shifting.

These Bandages may be washed, and always kept sanitary.

No.		Code	Price
854	3" width	<i>Elband</i>	Yard \$0.30
856	2" width	<i>Vanire</i>	" .20

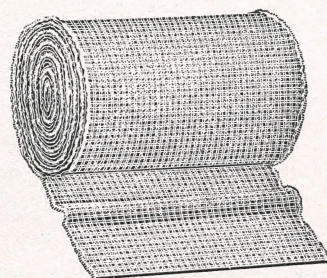

No. 854

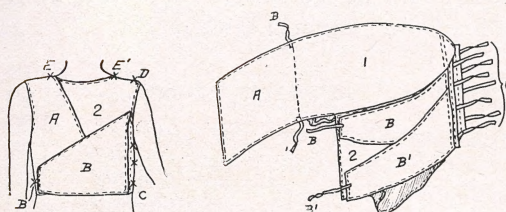The Lurie Diathermy Binder

The Lurie Diathermy Binder is constructed to minimize most of the disagreeableness of treatments by diathermy about the chest or abdomen, and to overcome the dangers of breaking contact.

No.		Code	Price
940	Lurie Cloth Binder	<i>Wintry</i>	\$2.50
941	Lurie Rubber Air Bag	<i>Wisdom</i>	3.00
942	Lurie Bag Inflator	<i>Wisely</i>	1.00
945	Lurie Binder Package, consisting of:		
	2 No. 940 Binders		
	2 No. 941 Air Bags (Rubber)		
	1 No. 942 Inflator	<i>Wisful</i>	10.00


Liquid Bath Connector

For carrying the Sinusoidal or Diathermy Currents to water in trays, for treating the limbs. Connector lays flat in the fluid, and wire connection is made to binding post.

No.		Code	Price
618	Liquid Bath Connector	<i>Gleam</i>	\$0.70

Sheet Block Tin

Sheet Block Tin, made specially flexible for use as Diathermy Electrodes, 12 inches wide, and in two thicknesses: .010 and .018 inch.




This is something entirely new in sheet electrode material, composed of a center of very flexible alloy with a sheet of pure tin on each side. Electrotherapists will appreciate the fact that pure tin is placed in contact with the skin in preference to the lead ordinarily supplied. It is easily cut with scissors.

Approximately one square foot of the .018 material, or two square feet of the .010 thickness, equals one pound.

No.		Code	Price
840	.010 thick	<i>Nessus</i>	Pound, \$0.65
841	.018 thick	<i>Nestle</i>	" .65

Electrode Clamp


No.		Code	Price
853	Electrode Clamp. Heavily constructed, with pliable rubber covering	<i>Winder</i>	\$0.35

**Electrode Clips**No. 868
Electrode Clamp

No.		Code	Price
868	Block Tin or Mesh Electrode Clamp	<i>Nettle</i>	\$0.30
852	The "Fahnstock" Clip	<i>Faconn</i>	.10

The Fischer No-Slip Contact Holder

Positively binds the Fischer Diathermy Cord and the No. 868 Clip together. Connection cannot pull apart.

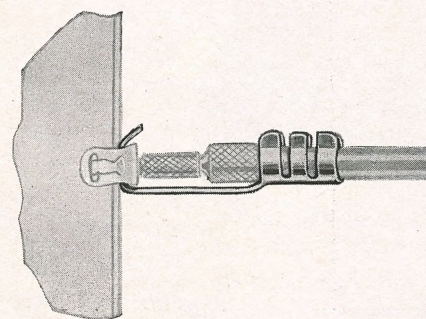


No.		Code	Price
869		<i>Wimper</i>	\$0.10





Disc Diathermy Electrodes

For the application of the Diathermy High Frequency Current. Discs are made of $\frac{1}{16}$ inch sheet brass, heavily nickel plated. Discs Nos. 606, 609, 625, 626, 627 and 628 are interchangeable on the same set of rubber handles. No handles are necessary with Nos. 610 and 611.

Small Size Discs			
No.		Code	Price
625	$\frac{3}{8}$ " diameter	Velour	\$0.45
626	$\frac{1}{2}$ " diameter	Velvet	.50
627	$\frac{3}{4}$ " diameter	Vendee	.55
628	1" diameter	Vendow	.70
630	Complete set of four above discs and handle	Vencer	2.50




Large Size Discs			
No.		Code	Price
606	2" diameter	Jaw	\$0.85
609	3" diameter	Graft	1.45
610	4" diameter	Grain	1.90
611	5" diameter	Gurgl	2.20
606R	Rubber Handle	Jecur	.70




New Fischer Diathermy Cords

Diathermy Cords are constantly getting wet, and when covered with a mercerized or silk webbing they are usually stained and discolored after but a few days' use.


Here are our much improved Diathermy Cords, covered only with pure gum rubber. They are very flexible, easily kept as clean as when new, and constructed to give long service.



No. 1330




No. 1332



No. 1334

No.		Code	Price
1330	6-foot cords, with heavy rubber insulation	Negro	Pair \$2.75
No.		Code	Price
1333	6-foot cords, with light rubber insulation	Wilful	Pair \$2.45
No.		Code	Price
1331	With special tips, for the Fischer Senior "FO," "LO," "G" or "GP" Diathermy Outfits	Wiciup	Pair \$2.75
No.		Code	Price
1332	Rubber-covered Diathermy Cord with special tip for Type "V" Outfit	Waiste	Pair \$5.50
No.		Code	Price
1334	Rubber-covered Diathermy Cords with right angle tip for "G2" Outfit	Warmih	Pair \$3.20


Diathermy Hand Electrode

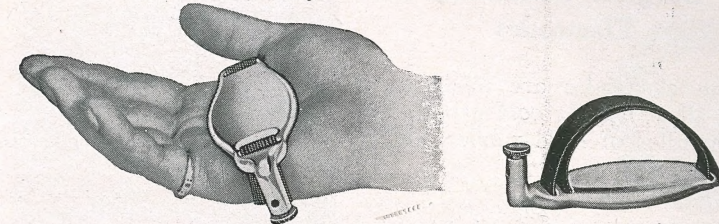


A most convenient method of applying the Diathermy Current by the hand, for local treatments. The rubber band holds the plate in close contact with the palm of the hand, and allows a free movement of the fingers for massage purposes. Carefully designed; all edges smoothly rounded and polished, making it an ideal and extremely convenient appliance.

No.		Code	Price
614	Hand Electrode	Grace	\$1.70

Flexible Pad Electrodes



No. 613

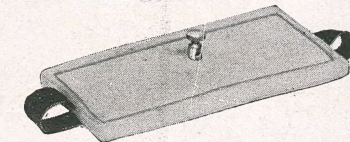


No. 690

A flexible, Felt Pad, backed with pure block tin. Can be adapted to most any shape. Has connection on back for fastening wire from machine.

No.		Code	Price
613	Felt Pad Electrode—8"—Round	Giddy	\$2.35
690	Felt Pad Electrode—3"x6"	Lasher	1.25

Pad electrodes of odd sizes and shapes, made to order. Write us your requirements.

A "Finger Rheostat" Fulguration Device

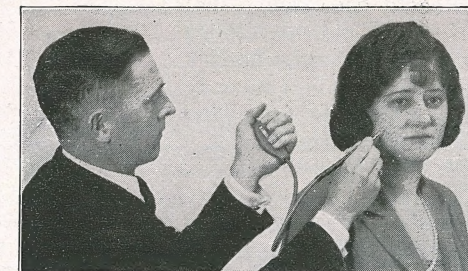


An innovation for the application of Fulguration Current via the indirect method. An insulated control is strapped to the left hand, enabling the operator to draw more or less current from the patient, at will, during the treatment. In the right hand is held the insulated handle and fulguration point. A finger rest is also provided.

No.		Code	Price
860		Safly	\$5.00

Surgical Diathermy Electrodes

The electrodes are made of a hard alloy, heavily *gold* plated, and the handles of hard rubber, highly polished.

- No.
1300 Complete set Gold Plated Surgical Diathermy Electrodes, with protected Cord and rubber Handles, as illustrated, in plush lined leatherette-covered Case.

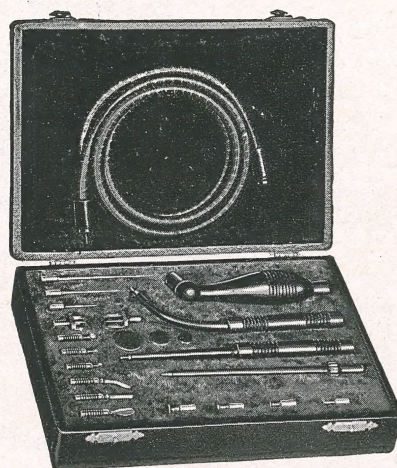


Code, *Macabe*. Price, \$75.00

No. 1300


No.		Code	Price
1301	Case, only, for set Surgical Diathermy Electrodes	<i>Macaco</i>	\$10.00
1302	Pharyngeal Electrode Handle.....	<i>Macard</i>	9.00
1303	Pharyngeal Electrode Holder	<i>Macaaw</i>	5.40
1304	Curved Handle	<i>Macduf</i>	3.90
1305	Straight Handle	<i>Machet</i>	3.00
1306	High Tension Cable—6' length.....	<i>Macerl</i>	3.70
1307	Single Needle Electrode (short).....	<i>Mackle</i>	1.70
1308	Single Needle Electrode (medium).....	<i>Macron</i>	3.30
1309	Single Needle Electrode (long).....	<i>Macula</i>	2.40
1310	Multiple Needle Electrode (short).....	<i>Madcap</i>	5.40
1311	Multiple Needle Electrode (long).....	<i>Madder</i>	5.40
1312	Knife Electrode (Cumberbatch)	<i>Madera</i>	2.85
1313	Blunt Knife Electrode (curved).....	<i>Madona</i>	2.96
1314	Blunt Knife Electrode (straight).....	<i>Madras</i>	2.20
1315	Button Electrode (small).....	<i>Maffia</i>	1.65
1316	Button Electrode (medium)	<i>Magian</i>	1.65
1317	Button Electrode (large)	<i>Maguey</i>	1.75
1318	Disc Electrode— $\frac{1}{8}$ " diameter.....	<i>Mahout</i>	1.65
1319	Disc Electrode— $\frac{3}{16}$ " diameter.....	<i>Maigre</i>	1.40
1320	Disc Electrode— $\frac{1}{4}$ " diameter.....	<i>Mainor</i>	1.25
1321	Disc Electrode— $\frac{3}{8}$ " diameter.....	<i>Majuba</i>	1.45
1322	Disc Electrode— $\frac{1}{2}$ " diameter.....	<i>Malaga</i>	1.40
1323	Disc Electrode— $\frac{3}{4}$ " diameter.....	<i>Malice</i>	1.90
1324	Disc Electrode—1" diameter	<i>Malign</i>	2.60

Physicians interested in Surgical Diathermy should read our free pamphlet, "Principles of Surgical Diathermy. Ask for Form 646.


New Surgical Diathermy Electrodes

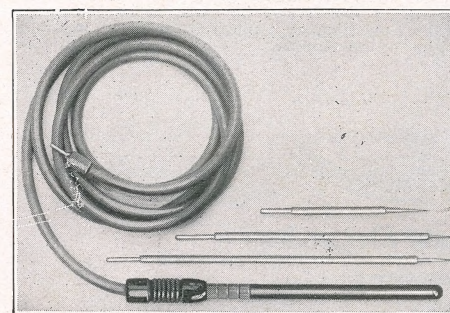

No. 862

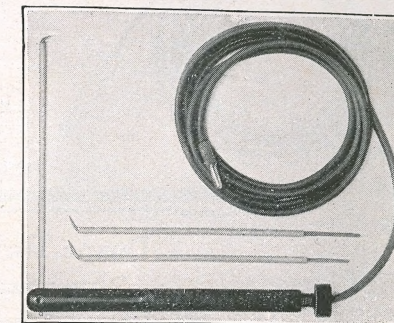

No. 920

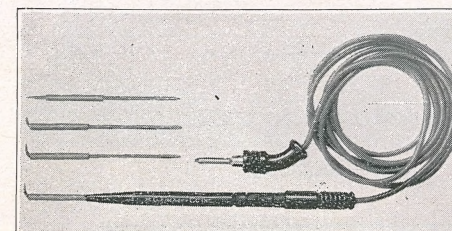


No. 740

Suggested by Drs. T. Howard Plank, D. Frank Knotts and Gregg Dillinger for electrocoagulation operations—especially tonsillectomies. They are small, light in weight and exceptionally handy for this work. The operator's hands are out of the line of vision, entirely, when making the application.

A very flexible rubber-covered cable is securely fastened directly into the polished hard rubber handle, and is sufficiently insulated that it may be wound around the hand and arm, or allowed to lay against the face of the patient with absolutely no danger of shocking.

There is no exposed metal anywhere, with the exception of the active tip. Tips of different lengths are furnished, as illustrated.

No.		Code	Price
862	The Plank Electrode and 3 tips.....	<i>Sally</i>	\$5.00
920	The Knotts Electrode and 3 tips.....	<i>Waylay</i>	10.00
740	The Dillinger Electrode, as illustrated, with 4 tips, constructed with special chuck in handle to prevent needles from turning	<i>Aide</i>	10.00

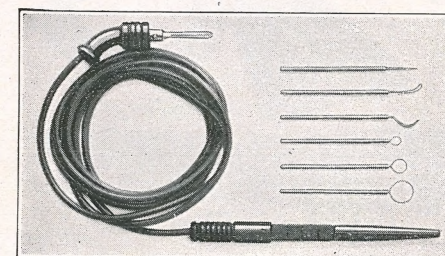

No. 791

This set of loops and knives with the special short insulated handle, is especially designed for tissue cutting purposes. Handle has special chucking device, preventing cutting instrument from turning during operation.


No.		Code	Price
791	Tissue Cutting Handle, with Cord and set of Tips as illustrated	<i>Wrasse</i>	\$10.00

"PILLAR RETRACTOR—DOUBLE END"

"Made of polished hard rubber. For use in connection with the electrocoagulation of tonsils.

No.		Code	Price
924	Dillinger Double - End Pillar Retractor	<i>Acedil</i>	\$2.50

No. 924

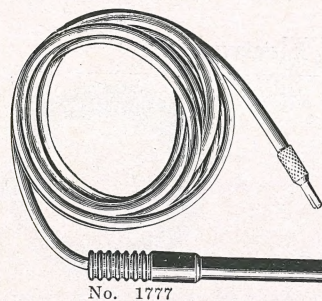

Adjustable Reaction Electrode

The metal electrode running through the center of the hard rubber sheath may be extended beyond the end of the insulation, or withdrawn into the sheath with a turn of the handle.

No.	Code	Price
1777	Scythe	\$5.00


Doane Turbinate Electrodes



No.	Code	Price
1785 Spade Shape	Warped	\$1.25
1786 Fork Shape	Warren	1.25
1787 Set of 2 Doane Electrodes as above	Warsaw	2.50

(Dr. Doane's "Turbinate Technic" will be sent on request)

The Thometz Tonsil Electrodes



No.	Code	Price
910 Thometz Electrodes (set of 3)	Thoset	\$4.00
911 Retractor and Handle	Thoret	1.40
912 4-Prong Electrode	Thofor	1.40
913 2-Prong Fork Electrode	Thotwo	1.40

(The No. 862 Plank Handle must be used to hold Nos. 912 and 913)

"Physiotherapy in Eye, Ear, Nose and Throat Conditions" is described in our folder Ask for Form 901

The Fischer Electrocoagulation Foot Switch

As illustrated, this Foot Switch lays close on the floor. A touch of the toe makes and breaks the contact.


It is molded of Bakelite and sufficient insulation has been used to make it shock proof. It is easily moved about, yet keeps an upright position on the floor.

The cable is very flexible, and covered with pure gum rubber; it may be washed and kept as new always. Cable terminals will be furnished to fit any style apparatus; specify machine used, when ordering.



Catalog No. 1498

No.	Code	Price
1498 Fischer Electrocoagulation Foot Switch, with 8-foot cable	Waving	\$10.50
1206 Extra rubber covered cable	Tiberi	Per foot .15

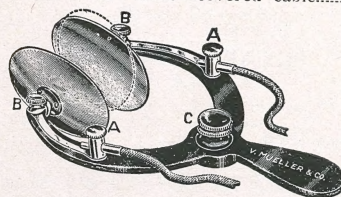

Epididymis Electrode

A specially designed clamp arrangement for administering diathermy current.

No.	Code	Price
1277 Epididymis Electrode	Corepi	\$12.00

Use of Diathermy in Epididymitis is described in our pamphlet. Ask for Form 530

Autocondensation Handles



No. 52



No. 58

Handle No.	Diam.	Length	Code	Price
52	1"	9"	Carota	\$1.20
81	1"	10"	Vitals	2.00
58	1½"	14"	Authan	3.00

Autocondensation Couch Cushion




Cushion is made of sea moss covered with black DuPont Fabrikoid material with an electrode of zinc.

The Fischer cushion is fully two and one-half inches thick. Size over all, 22 inches wide and 62 inches long.

No.	Code	Price
420 Auto Couch Cushion	Caffea	\$33.00

Autocondensation Couch Pad

A well made pad of black DuPont Fabrikoid material measuring 22 inches wide by 62 inches long. The insulating material between the patient and the center electrode plate is oiled silk and wool felt. The entire pad is about ¾ inch thick and is designed for machines of medium voltage d'Arsonval output, as for example the Fischer Type "G2" Diathermy Outfit.



No.	Code	Price
418	Cadogg	\$30.00

Special G. U. Auto Pad



An autocondensation pad of precisely the same dimensions as catalog No. 418 but split as illustrated. This style of pad was originally designed and used

by Dr. B. C. Corbus in his G. U. Diathermy work.

No.	Code	Price
416 Corbus Auto Pad	Corpad	\$30.00

See our pamphlet, "Treatment of Gonorrheal Endocervicitis by Heat" Ask for Form 571

Autocondensation Chair Pad

No. 410

Frame made of five-ply veneered oak. On one side is mounted a layer of conducting metal covered with a dielectric of one-eighth inch black sheet fiber.

No. 410 Chair Pad *Cado* \$10.00
 No. 413 Flexible Chair Pad of approximately the same size and shade as No. 410, but made of same material and in the same manner as No. 418 on opposite page. *Viatric* \$10.00



No. 413

Wooden Treatment Table

A solid, well made treatment table of all-wood construction, finished in mahogany. Has a compartment under the top for storing the autocondensation pad when not in use.


No. 422 *Tettat* \$75.00

Rowell Urethral Electrode Set


For treatment of gonorrhea in the male. For full information as to Dr. Rowell's technic, ask for descriptive pamphlet.

Rowell Urethral Electrode; straight perforated electrode of metal; nickel plated, for internal urethral treatments; Bakelite Frame with Clamps and Thermometer (Luer Syringe not included.)

No. 1372 *Vortex* \$25.00

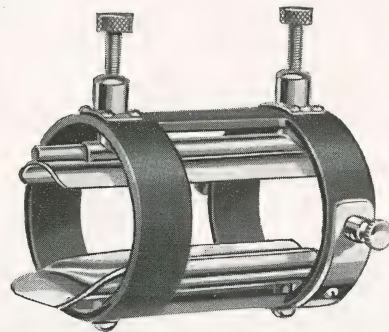**Thermometer for Rowell Electrode**

No. 1373 *Waddie* \$2.50
 For Rowell Electrode No. 1372

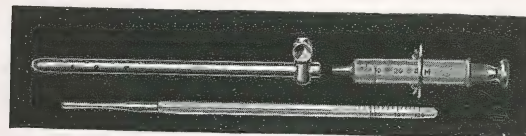**The Chapman Vaginal Electrode**

Designed along scientific lines, with size and shape of polished metal end to properly engage the lips of the cervix. The shank, or handle, is made of hard rubber. This electrode is to be used with Diathermy Current. Supplied both with and without the special thermometer which permits the accurate maintenance of an exact temperature within the vagina. This instrument is of extreme value in the treatment by diathermy of painful or inflammatory conditions of the female pelvis.




No. 1885. Chapman Vaginal Electrode—Side View



No. 1885. Chapman Vaginal Electrode—Top View



No. 1886. Chapman Vaginal Electrode with Special Thermometer

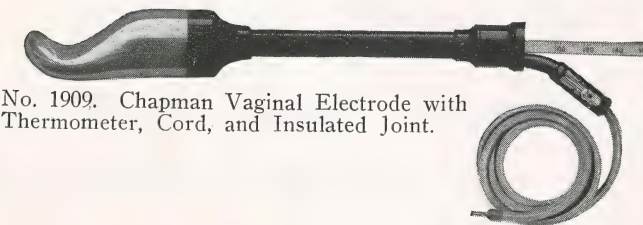

No. 1909. Chapman Vaginal Electrode with Thermometer, Cord, and Insulated Joint.

No.		Code	Price
1886	Regulation size, with thermometer. Shank $1\frac{1}{8}$ " diameter, cervical bowl $1\frac{3}{4}$ " wide and $\frac{3}{8}$ " thick. Handle of hard rubber.....	<i>Chavag</i>	\$13.00
1885	Regulation size, without thermometer arrangement.....	<i>Chapel</i>	6.75
1884	Small size, with thermometer. Shank $\frac{1}{8}$ " diameter, cervical bowl $1\frac{1}{8}$ " wide, $\frac{1}{8}$ " thick. Hard rubber handle.....	<i>Chasma</i>	13.00
1883	Small size, without thermometer arrangement.....	<i>Chalit</i>	6.75
1909	Regulation size, as No. 1886, with thermometer and with cord and insulated joint.....	<i>Vermin</i>	16.00
1907	Small size, as No. 1884, with thermometer and with cord and insulated joint.....	<i>Verity</i>	16.00

Technic for the Chapman Vaginal Electrode is fully described in our pamphlet, "Diathermy in Gynecology." Ask for Form 643.

Copper Intra-Uterine Electrodes

Three sizes. The smallest size end is all copper, and the medium and large sizes have hard rubber tips.



No.		Code	Price
1834	Small Copper End on Rubber Shank.....	<i>Nentul</i>	\$3.50
1835	Medium size Copper End with Hard Rubber Tip.....	<i>Nonter</i>	3.50
1836	Large size Copper End with Hard Rubber Tip.....	<i>Neural</i>	3.50
1838	Set of 3 Electrodes as above.....	<i>Neuter</i>	10.00

Urethral

No.		Code	Price
1860	Hard Rubber Holder with Copper Tip $\frac{1}{8}$ " diameter.....	<i>Nigrit</i>	\$3.00
1861	Hard Rubber Holder with Copper Tip $\frac{1}{8}$ " diameter.....	<i>Varix</i>	3.00
1862	Hard Rubber Holder with Copper Tip $\frac{1}{4}$ " diameter.....	<i>Niobee</i>	3.00
1863	Hard Rubber Holder with set of 3 tips as above.....	<i>Nipper</i>	3.75
1864	Hard Rubber Holder, only.....	<i>Nisann</i>	1.50
1865	Copper Tip only, $\frac{1}{8}$ " diameter.....	<i>Noddle</i>	1.00
1866	Copper Tip only, $\frac{1}{8}$ " diameter.....	<i>Noetic</i>	1.00
1867	Copper Tip only, $\frac{1}{4}$ " diameter.....	<i>Nodose</i>	1.00





No.		Code	Price
1870	Hard Rubber Holder with Copper Olive Tip, 17F dia.....	<i>Nissus</i>	\$2.00
1871	Hard Rubber Holder with Copper Olive Tip, 20F dia.....	<i>Nitrat</i>	2.00
1872	Hard Rubber Holder with Copper Olive Tip, 23F dia.....	<i>Nitros</i>	2.00
1873	Hard Rubber Holder with Copper Olive Tip, 25F dia.....	<i>Nivose</i>	2.00
1874	Hard Rubber Holder with set of 4 Olives as above.....	<i>Nobody</i>	3.30
1875	Hard Rubber Holder, only.....	<i>Nocent</i>	1.50
1876	Copper Olive only, 17F diameter.....	<i>Nogin</i>	.65
1877	Copper Olive only, 20F diameter.....	<i>Nonact</i>	.65
1878	Copper Olive only, 23F diameter.....	<i>Noncom</i>	.65
1879	Copper Olive only, 25F diameter.....	<i>Nonego</i>	.65
1880	Perforated Hard Rubber Olive, for Cataphoresis, with Holder.....	<i>Noodoo</i>	2.25
1881	Perforated Hard Rubber Olive only.....	<i>Norman</i>	.75

The Fischer-Funk Penile Electrode

Admirably adapted to the Diathermy treatment of gonorrhea (male). The salt water level is altered by depressing or releasing the rubber reservoir bulb. Furnished complete as illustrated.

No.	Code	Price
1890	<i>Funkel</i>	\$11.00

See our free pamphlet, "Treatment of Genito-Urinary Diseases with Diathermy," by Dr. Funck. Ask for form 668.

**Carbon Ball**

No.		Code	Price
1821	Carbon Ball Electrode.....	<i>Marcus</i>	\$2.00

Oblong Copper Ball

No.		Code	Price
1822	Oblong Copper Ball Electrode.....	<i>Margay</i>	\$2.50

Sigmoid


No.		Code	Price
1823	Sigmoid Electrode—aluminum tip.....	<i>Marine</i>	\$3.00

Prostatic

No.		Code	Price
1824	Prostatic Electrode—aluminum tip.....	<i>Marmo</i>	\$2.50


Vaginal

No.		Code	Price
1825	Vaginal Electrode—aluminum tip.....	<i>Marlin</i>	\$3.75

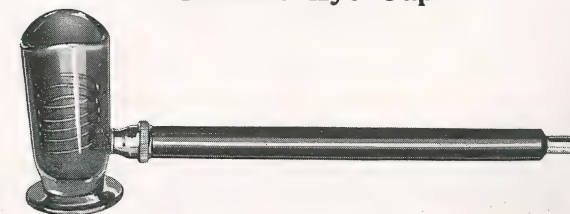Galvanic Eye Cup


No.		Code	Price
1830	Eye Cup (for Galvanism).....	<i>Marly</i>	\$3.90

Interrupter Handle With Moist Pad

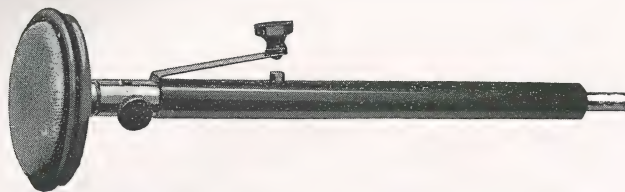


No.		Code	Price
1831	Interrupter Handle with Moist Pad.....	Mashe	\$5.50

Cataphoric

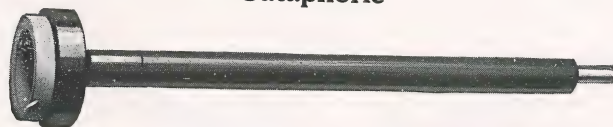

No.	Electrode with Rubber protection and Carbon base.	Code	Price
1832	Cataphoric Electrode	Mason	\$6.25

Flexible Sigmoid



Electrode, constructed of pure block tin tubing, with hose end for flushing attachment.

No.		Code	Price
1833	Flexible Sigmoid Electrode.....	Massa	\$3.00

New Two Pole Electrodes

For treating localized conditions in the rectum and vagina.

Rectal



No.		Code	Price
1852	Rectal Electrode	Masree	\$8.00


Vaginal



No.		Code	Price
1853	Vaginal Electrode	Masvag	\$8.00

Fischer Moist Pad Electrodes


Formed of an asbestos compound which is thoroughly water soaked before applying. Covered with heavy white linen fabric. The metal electrode plate is sewed snugly to the pad, and contact with the connecting cord is made with the Fischer Flat Spring Connection.

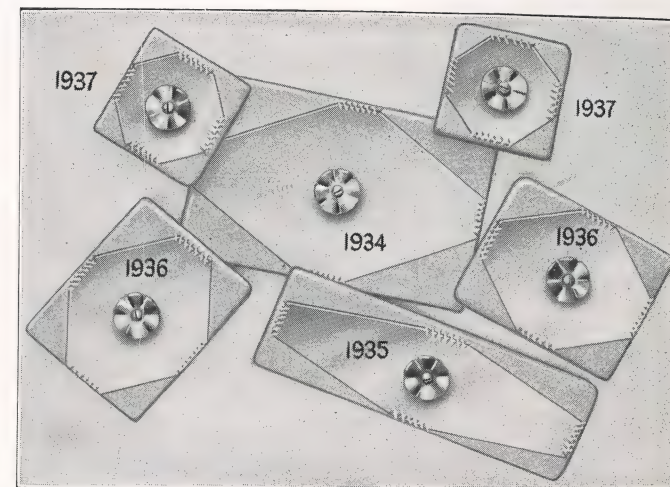


No.		Code	Price
1934	Flat Pad Electrode for No. 1125—5x8".....	Wapiti	\$2.00
1935	Flat Pad Electrode for No. 1125—3x9".....	Warble	1.70
1936	Flat Pad Electrode for No. 1125—4x5".....	Warden	1.70
1937	Flat Pad Electrode for No. 1125—3x3".....	Warily	1.60

Fischer Diathermy Belt Electrode

Composed of a series of aluminum rectangular cups, linked together, and a flexible rubber belt. One or more electrodes (cup) may be employed for applying diathermy to any small area, or as many links as may be required to pass around the entire abdomen; especially useful in connection with internal electrodes as the indifferent plate. Twenty-two cups to set.

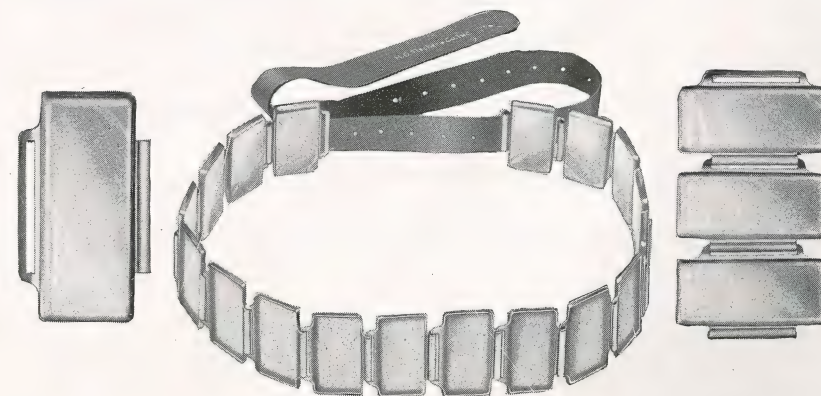


No.		Code	Price
1888	Belt Electrode, 22 cups and rubber belt.....	Dibelt	\$18.00

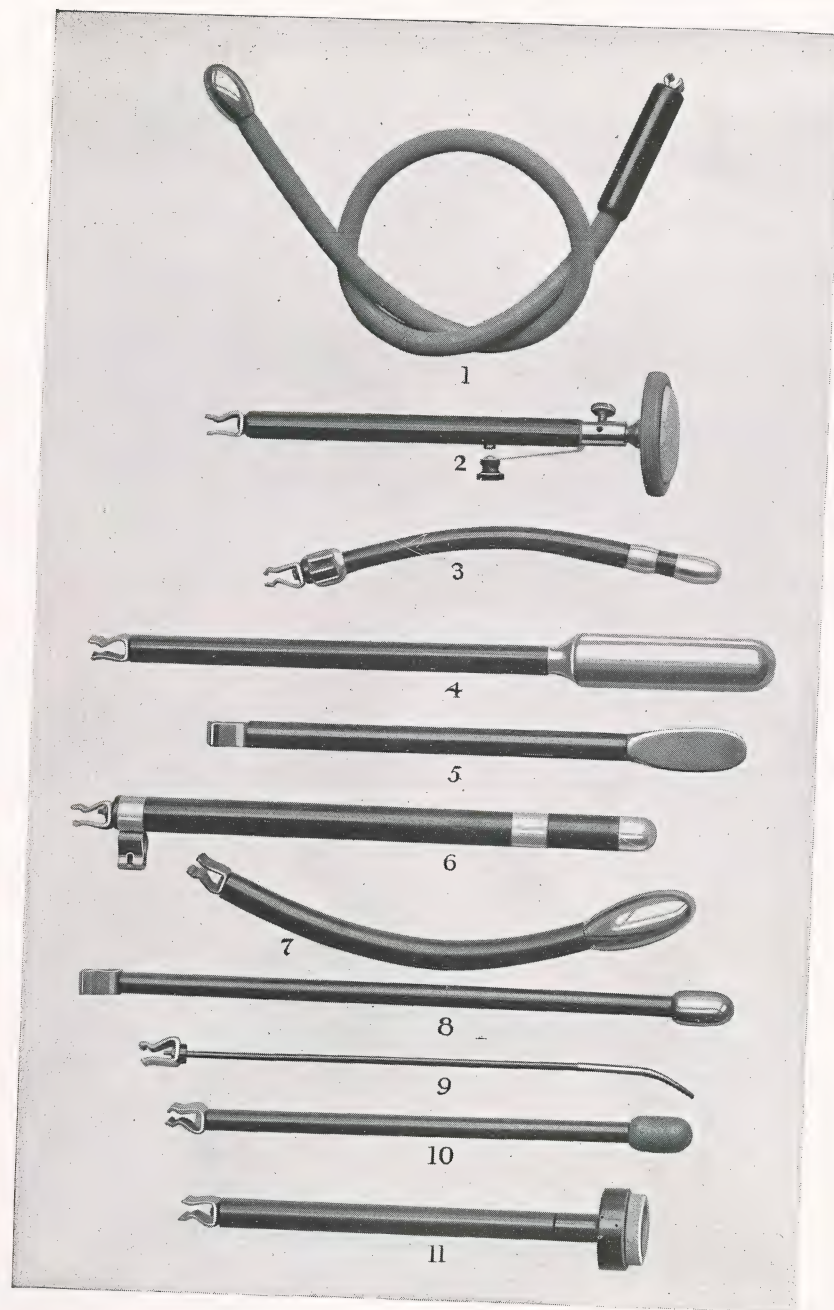

Internal Electrodes

These electrodes are essentially the same as those illustrated and described on pages 23 and 24, except that the connectors are of the "Morse" type to accommodate cords furnished with the Morse Wave Generator.

No.		Code	Price
1940	Flexible rectal electrode, for localized muscle exercise to high rectal area as in constipation at region of descending colon, to splenic flexure. (No. 1).....	Unhat	\$6.50
1941	Diagnostic electrode, for electro diagnosis (muscle testing) to determine degree of local disability. (No. 2).....	Union	5.50
1942	Bi-polar rectal electrode, for local invigoration of relaxed rectal region. (No. 3).....	Unles	8.00
1943	Vaginal electrode, for general invigoration of pelvic organs (relaxed conditions.) (No. 4).....	Unlok	3.75
1944	Prostatic electrode, to massage rhythmically, by muscle contraction (sine wave current). (No. 5).....	Untie	2.50
1945	Bi-polar vaginal electrode, for local invigoration of vagina (relaxed conditions). (No. 6).....	Upend	8.00
1946	Sigmoid electrode, for constipation due to prolapsed descending colon and sigmoid impaction. (No. 7).....	Uphil	3.00
1947	Oblong copper ball, for local astringent effect on mucous surface as in leucorrhoea, bleeding hemorrhoids, etc. (No. 8).....	Upset	2.50
1948	Intra-uterine electrode, copper, with hard rubber tip, for treatment of endometritis and control of uterine hemorrhoid (positive pole), stenosis of cervix (negative pole). (No. 9).....	Urase	4.25
1949	Oblong carbon ball electrode, for relief of inflammation and relaxed conditions of the uterus and vagina (positive pole). (No. 10).....	Uredo	2.00
1950	Cataphoric electrode, to introduce medicates, using galvanic current. (No. 11).....	UriaH	6.75

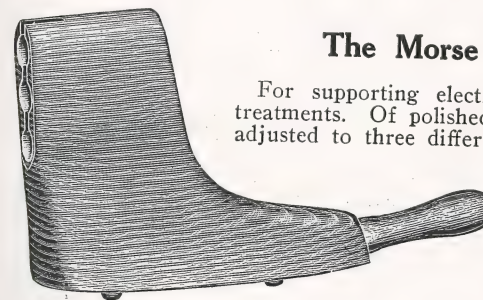


The Morse Electrode Support

For supporting electrodes during rectal and vaginal treatments. Of polished hard wood. Electrodes may be adjusted to three different heights.

No.		Code	Price
1854	Morse "Shoe" Electrode Support	Moshoe	\$8.75

Carbon Hemorrhoid Electrodes

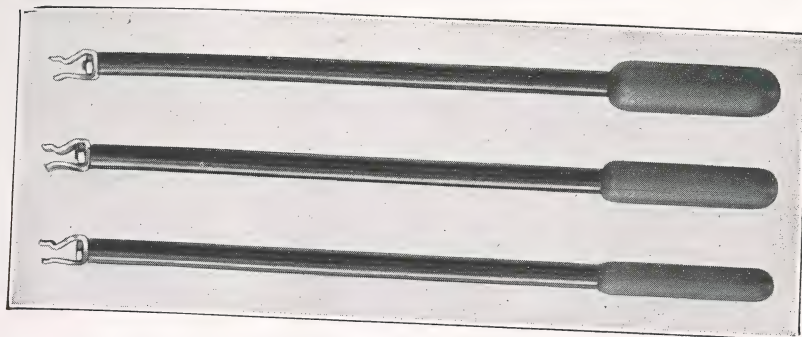


For astringent effect, positive pole.

This set of electrodes is furnished in three sizes, where the smaller electrode may be more easily inserted during early treatment, using subsequently the two large ones.

No.		Code	Price
1951	Carbon electrode—small	<i>Uriel</i>	\$2.75
1952	Carbon electrode—medium	<i>Urpod</i>	3.00
1953	Carbon electrode—large	<i>Ursan</i>	3.25

Small Muscle Testing Pads

Pads Nos. 1846, 1847 and 1848 are made with metal backing with asbestos as the absorbent material, and covered with linen.



No. 1846

Nos. 1895, 1896 and 1897 are made of metal with a chamois covering over the ball end.




No. 1898

No.		Code	Price
1846	With pad $\frac{5}{16}$ "x $1\frac{3}{4}$ "	<i>Nictat</i>	\$0.85
1847	With pad $\frac{3}{8}$ "x $1\frac{3}{4}$ "	<i>Niello</i>	.85
1848	With pad $\frac{1}{2}$ "x $1\frac{3}{4}$ "	<i>Niever</i>	.85
1850	Set of 3 as above	<i>Niggle</i>	2.50
1895	Localizing Electrode (Small)	<i>Valet</i>	.75
1896	Localizing Electrode (Medium)	<i>Valid</i>	.80
1897	Localizing Electrode (Large)	<i>Valor</i>	.85
1898	Set of 3 Ball Electrodes	<i>Varie</i>	2.40

Fischer-Morse Cord-Electrode Adapter

Necessary when employing the cords furnished with the Morse Wave Generator in connection with any of the Fischer Internal Electrodes.




No.		Code	Price
1858		<i>Morada</i>	\$0.45

Galvanic Needle Holder


Made of hard rubber with nickel-plated metal clamp.

No.		Code	Price
1900	Galvanic Needle Holder	<i>Myope</i>	\$2.50
1901	Galvanic Needles (12 in glass tube)	<i>Myrrh</i>	1.25

No.		Code	Price
1902	Hayes Bulbous Pointed Steel Needles	<i>Weasel</i>	\$2.50




No. 1904

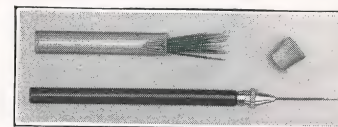

Nos. 1900 and 1901


No.		Code	Price
1904	Rubber covered Galvanic Cords, 2 colors—red and gray	<i>Mycor</i>	\$1.70

Rubber-Covered Connecting Wires



No. 1930

No.		Code	Price
1930	Pair Rubber-covered Connecting Wires with flat terminals, for Fischer Low Voltage Generator No. 1125. Code <i>Wander</i> , Price \$3.90		
1931	Pair Rubber-covered Connecting Wires with tips for Fischer Low Voltage Generator No. 1125. Code <i>Wanton</i> , Price \$3.40		



No. 1931

No.		Code	Price
1933	Bifurcated Cord with flat terminals for No. 1125	<i>Warned</i>	\$3.50

Spongio Discs and Handles




Universal Handle, hard rubber, with Felt covered disc.


No.		Code	Price
314	Felt Covered Disc	<i>Carsid</i>	\$0.40
315	Hard Rubber Handle	<i>Carhan</i>	.70
316	Felt Pad Disc and Handle	<i>Carmin</i>	1.30

Treatment Cords

Made of very flexible Copper stranded wire, covered with a mercerized sheathing, maroon colored. Have metal tips on both ends.

No.		Code	Price
312	Cords	<i>Carol</i>	\$0.75





Metal Treatment Handles

Nickel-plated handles, for Sinusoidal, Galvanic and Faradic treatment.

No.	Code	Price
311 Handles, pair	Caries	\$1.00

The Hawkeye Timer


Registers the length of any treatment exactly. A wonderful aid to accurate timing, particularly valuable when the physician is treating more than one patient at a time. The Hawkeye rings an alarm at the exact moment treatment should end. Should be in every treatment room.

No.	Code	Price
469 Hawkeye Timer	Vestry	\$7.50



L-F Treatment Timer

For Timing X-Ray, Diathermy, Quartz Lamp, Radiant Heat Lamp Treatments.—One minute to one hour. Automatically rings a gong and cuts off current at expiration of time. Setting can be tested, but switch will not remain on unless timer is set. Has Set-Back feature. Pointer can be overset, then turned back to exact time desired. *Automatically Integrating*—The Timer Switch can be turned on or off as often as desired during treatment. It will then automatically sum up the different periods of actual treatment. Operates on any X-ray machine equipped with magnetic switch. On Mercury Vapor or Radiant Heat Lamps, eliminates accidentally leaving lamp burning over night. *Safe*—Patient can at any time instantly turn off current by means of emergency pull cord held in hand.


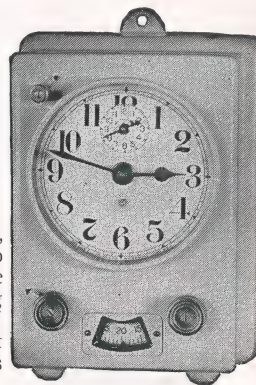


No.	Code	Price
370 L-F Treatment Timer.....	Wittles	\$35.00

Breuer Safety Switch

The terminals of this switch are made to fit the foot switch openings on all Fischer Diathermy Outfits. The switch operates with a pull cord, just like an electric light socket, so that either the physician or the patient may turn the current on or off in a moment. This switch gives patients a feeling of perfect safety.

No.	Code	Price
86 Breuer Safety Switch, complete with insulated pull cord.....	Varier	\$10.00

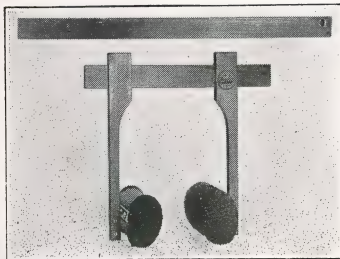


Clamp Electrode

You will note that the metallic material is placed over one sponge, only. The sponge on the opposite side is used to insure pressure contact. It may be applied and removed in an instant, and on practically any part of the body.

The three sizes of sponges on page 7, Nos. 891, 893 and 894 are interchangeable on this clamp. To be used with alternating and sine wave currents, but not for galvanism.

No.	Code	Price
931 Universal Clamp Electrode.....	Wealth	\$11.75

The Hollender-Cottle Headband and Electrodes

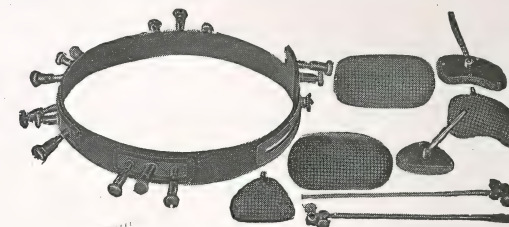

This perfected headband is a wonderful help to the physician in giving Diathermy for partial deafness, for nasal accessory sinus disease, and for nerve affections about the face. It is of use also for administering diathermy to the eye.

The outfit consists of the headband, with connections for electrodes, cords and electrode holders as illustrated.

Headband and electrodes are readily adjusted to give proper pressure in any combination of applications. In treating the ear, the indifferent electrode is placed on the face anterior to the opposite ear, while in treating the sinuses the indifferent electrode is placed on the nape of the neck.



No.	Code	Price
1360 Hollender-Cottle Headband with electrodes as illustrated and listed above.....	Veador	\$38.00
1361 Headband with Binding Posts only.....	Vector	25.00
1362 Long Electrode Support (2).....	Vedett	5.20
1364 Oval Electrode (2).....	Vedett	2.90
1365 Curved Electrode (2).....	Vellate	2.65
1366 Triangle Electrode (2).....	Vellum	2.45
1333 6 ft. Cords (2).....	Wilful	2.45

Also ask for our pamphlets, form No. 912 and form No. 913

Self-Retaining Ear Speculum

For Use in Metallic Ionization of Chronic Otorrheas

This simple apparatus obviates the necessity of holding the speculum in the ear canal. Furthermore, the indifferent electrode is on the inner side of the leather band, part of the same apparatus, doing away with large

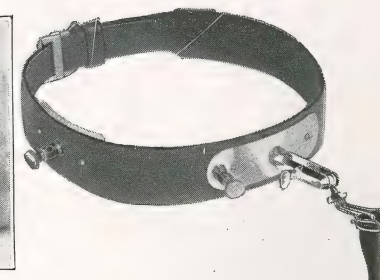

pad electrodes usually employed in this work and placed about the forearm or other surfaces of the body. The binding posts on the outer part of the headband serve for the connection of cords from the galvanic apparatus.

The leather band is easily placed around the head with the speculum directed into the ear canal to be treated. A free rotary motion of the speculum holder facilitates the direction of the rubber speculum so that no difficulty is encountered in setting it in proper position.

References—For the technic of metallic ionization in chronic otorrhea, see the following:

Friel, A. R., "The Treatment of Chronic Otorrhea in School Children," Hospital and Health Review, January, 1922.



Warwick, H. L., "Zinc Ionization in the Treatment of Chronic Suppurative Otitis Media," Texas State J. of M., October, 1923.

Hollender, A. R., and Cottle, M. H., "Physical Therapy in Diseases of the Eye, Ear, Nose and Throat," The Macmillan Co., 1926. (p. 66.)

No.	Code	Price
1355 Self-retaining Ear Speculum.....	Wassal	\$15.00

Biaural Cords

No.	Code	Price
1765 As illustrated	Wagcur	\$2.00

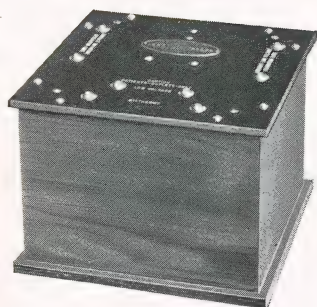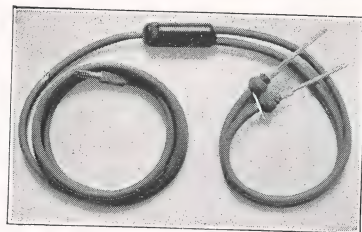

The Fischer Duplex Hi-Lo Volt Control


The object of this device is to enable the operator to administer simultaneously the Diathermy and Low Voltage or contractual currents.

A great time saver for the busy office or clinic. Any low voltage current, galvanism, sinusoidal or surging may be employed with the diathermy, cutting the treatment time in half.

Write for full particulars.

No.	Code	Price
1195	Hilovo	\$50.00

The Linn Ear Electrode and Control

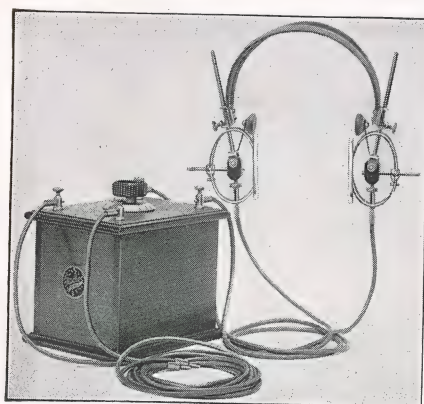

No. 1270 and No. 1272




The Linn Ear Electrode and Current Control is an innovation for diathermy treatment. The small control box enables the use of a very finely regulated current volume, independent of diathermy machine setting. The apparatus is complete, with headband, external U-shaped plates and cords, as illustrated.

No.	Code	Price
1270 Linn Biaural Electrode, complete, as illustrated, without control box.....	Lineal	\$15.00
1272 Linn Ear Electrode Control.....	Lincon	18.00

For use of the Linn Ear Electrode, see our free pamphlet. Ask for Form 705

The Kolischer Spark Gap

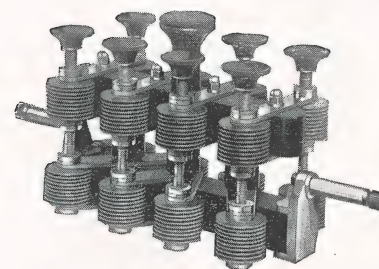

A vast improvement over any other type of Spark Gap ever devised for any high frequency machine.

This "Kolischer" Gap will fit the supports on any Fischer or Thompson-Plaster Styles "F" and "F-O" machines, as well as the Types "L,"


"L-O" and "Military" models without alterations or other attachments.

This new Multiple Spark Gap is equipped with 16 Tungsten spark interrupter points, adequate copper flanging to carry away all heat, and individual control for each set of tips as well as master controller for simultaneous adjustment. Quiet, perfect control is possible at any voltage or milliamperage, more constant discharge obtained at any setting, and the regulation is gradual—as compared to the usual jumps—the utmost in utility and flexibility.

No.	Code	Price
1222 Kolischer Spark Gap.....	Kolgap	\$75.00

The Baumanometer

An instrument of precise accuracy for measuring blood pressures. Especially valuable in connection with d'Arsonval Auto-condensation treatments. The Cartridge Tube of the new Lifetime Baumanometer is guaranteed against breakage for the original owner's lifetime! The straight glass tube with sturdy walls represents the utmost attainable simplicity and strength. Its smoothly ground ends and the cork-faced surfaces against which they bear are all accurately parallel, which insures a uniformly distributed pressure. The tube mounting is simple in construction, its resilient action absorbs the hardest jolts and jars.

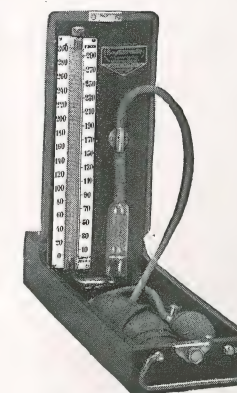


No. 436


No.	Code	Price
436 Desk Model	Baumon	\$36.00
437 Kit-Bag Model	Baukit	34.00
438 Pocket Model	Bapock	32.00
439 Wallboard Model	Bawall	30.00
440 Cabinet Model	Bacabi	43.00

Fischer High Frequency Milliampere Meters— D'Arsonval Type


For measuring D'Arsonval and Diathermy currents we have designed special meters of the true "D'Arsonval" type, registering to 5000 milliamperes.

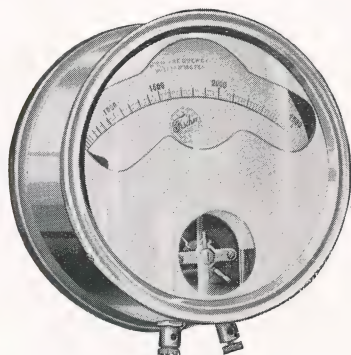

No. 450



No. 452



No. 454

No.		Code	Price
449	Calibrated from 0 to 1500 Milliamperes.....	<i>Exo</i>	\$30.00
450	Calibrated from 0 to 2500 Milliamperes.....	<i>Exoda</i>	30.00
451	Calibrated from 0 to 5000 Milliamperes.....	<i>Exner</i>	30.00
452	Calibrated 0 to 1000 (Mounted).....	<i>Exmoor</i>	25.00
Catalogue No. 452 is specially designed to set on a table, for use with portable machines or small cabinets not previously equipped with meter. Mounted in upright holder, making dial always visible.			

No.		Code	Price
454	Calibrated 0 to 1000—0 to 4000 (Double Scale). For types "G" and "G2" Fischer Portable Diathermy Outfits.....	<i>Extong</i>	\$30.00
456	Calibrated 0 to 1000—0 to 4000 M. A. (Double Scale). For Fischer Type "V" Cabinet.....	<i>Whydah</i>	25.00
462	Double Scale Meter for Senior "FO" and "LO" Outfits.....	<i>Varlet</i>	50.00

Fuse for Meter Protection

No.		Code	Price
457	Fuse as furnished with the Fischer Type "G2" Portable Diathermy Units	<i>Gefuse</i>	\$0.30

Insulating Oil for Transformers

When, for any reason whatever, the insulating oil in which your transformer is immersed needs replenishing, *never use ordinary lubricating material*. The proper oil must be mineral in substance, and capable of withstanding a very high flash test.


The safest procedure is to order the desired quantity from us, with the assurance that only that oil which is exactly correct will be sent you.

No.		Code	Price
725	Tested Transformer Oil, in 1 qt. can.....	<i>Trafil</i>	\$0.60
726	Tested Transformer Oil, in 1 gal. can.....	<i>Tanoil</i>	2.00

Tungsten Spark Interrupter Points

Steel bases faced with a heavy thickness of *pure tungsten* form points for spark interrupters that are almost everlasting, and will improve the action of any High Frequency apparatus not already so equipped.

Carried in stock in three sizes, as illustrated, both male and female.



No. 91

No. 89

No. 90

No.		Code	Price
89	$\frac{1}{4}$ inch diameter, as used on our DeKraft and Kolischer Gaps on the "F," and "F-O," "L," "L-O" and "Military" machines, each	<i>Tunpot</i>	\$0.75
90	$\frac{3}{8}$ inch diameter, as used on our Portable Types "K" and "G2," and the "E" and Eye, Ear, Nose and Throat Cabinets, pair	<i>Tuntyk</i>	3.50
91	$\frac{1}{8}$ inch diameter, as used on our Portable Type "F," each.....	<i>Tunfpo</i>	.50



Leyden Jars

Designed for use with our Types "FO," "LO" and Military High Frequency generators. Made of best quality glass, carefully coated.

No.		Code	Price
615	Leyden Jar, complete as illustrated (1 qt. size).....	<i>Hydat</i>	\$4.50
616	Leyden Jar, less Top and Carbon (1 q.t size).....	<i>Laurel</i>	3.70


Electrolytic Salt

Specially prepared for electrolytic purpose; one package of $\frac{1}{2}$ pound makes proper and full charge for our No. 615 Leyden Jar, illustrated above.



No.		Code	Price
879	$\frac{1}{2}$ lb. package.....	<i>Leysal</i>	\$0.12

High Frequency Electrodes

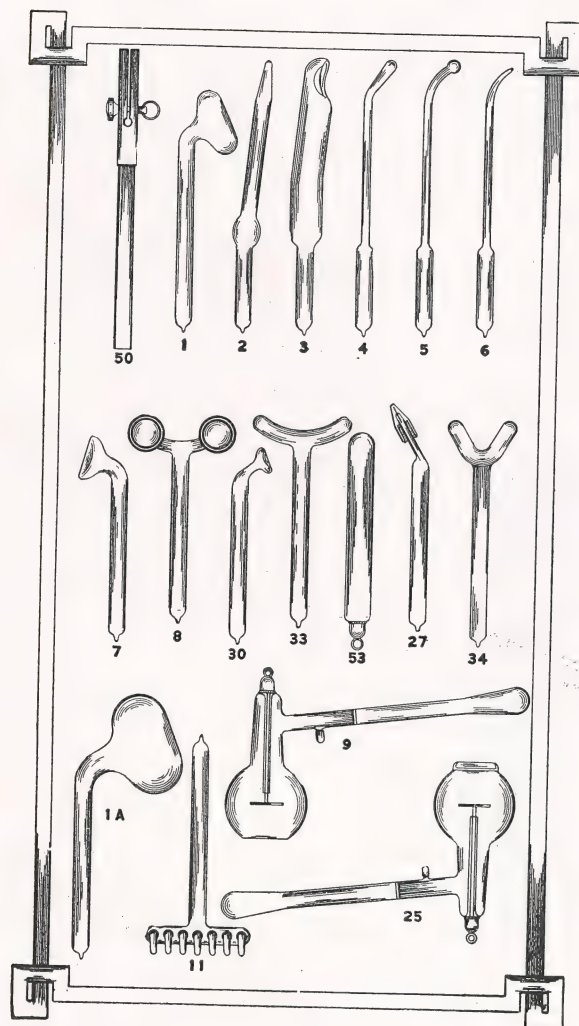

High Frequency Electrodes

All our glass High Frequency electrodes are made by us, of the very best glass obtainable; carefully annealed. All sizes and makes of holders can be fitted on request, but unless otherwise specified our standard $\frac{5}{8}$ " size is furnished on all orders.


The "O" before any number signifies $\frac{1}{2}$ " stem.

No.	Description	Code	Price
1—Surface	—Plain	<i>Bacca</i>	\$0.75
1A—Surface	—Plain	<i>Gram</i>	1.50
2—Rectal	—Plain	<i>Bagot</i>	.65
3—Vaginal	—Plain	<i>Ballet</i>	.85
4—Nasal	—Plain	<i>Balm</i>	.65
5—Throat	—Plain	<i>Baric</i>	.65
6—Urethral	—Plain	<i>Bark</i>	.65
7—Eye, Single	—Plain	<i>Barley</i>	.75
8—Eye, Double	—Plain	<i>Basal</i>	1.50
9—Metal Disc Body	Condenser Type	<i>Basic</i>	3.50
11—Comb (Scalp)		<i>Batia</i>	1.75
25—Cataphoresis		<i>Binder</i>	3.50
27—Glass Fulguration		<i>Guad</i>	1.75
30—Corn—Small Cavity		<i>Biogen</i>	.75
33—Outer Throat		<i>Biotic</i>	.90
34—Spinal		<i>Bite</i>	.75
050—Universal Handle, $\frac{1}{2}$ "		<i>Boldo</i>	1.30
50—Universal Handle, $\frac{5}{8}$ "		<i>Bolus</i>	1.30
53—Glass Handle for Indirect Treating		<i>Bismal</i>	1.75
56—Adjustable Handle		<i>Boman</i>	1.65


This perfected high frequency handle is made of hard rubber, with cord attached, ready for use with any standard $\frac{1}{2}$ inch electrode. No bare metal, no shocks, utmost convenience and comfort in treating patient.

No.	Price
059 Hollender-Cottle, Insulated adjustable, High Frequency Handle, complete with cord. Code, <i>Hocoin</i>	\$16.00

Hollender-Cottle Insulated Adjustable High Frequency Handle

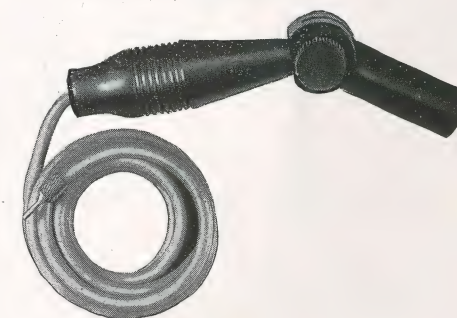

Insulated Glass High Frequency Electrodes

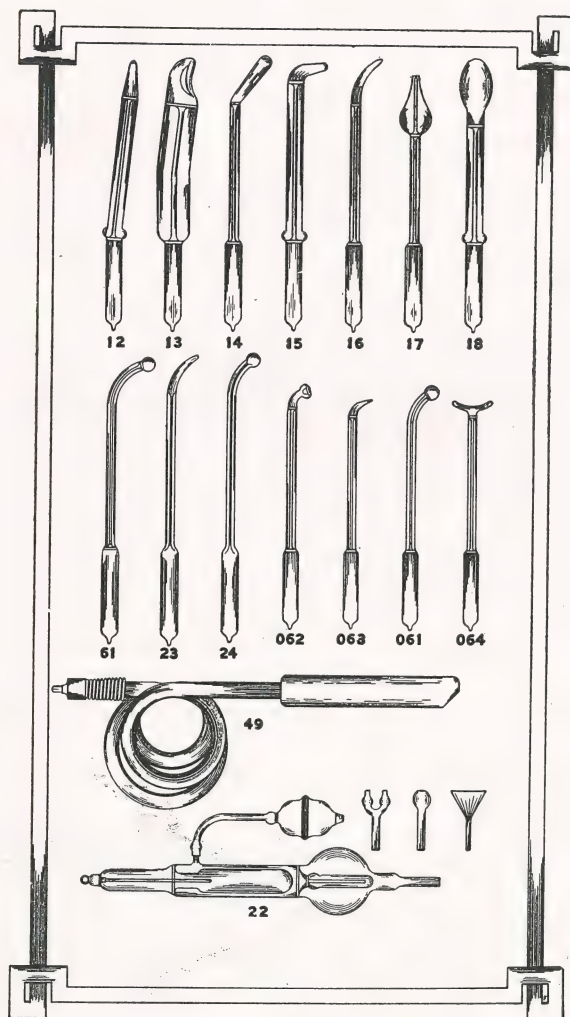

Insulated Glass High Frequency Electrodes

No.	Description	Code	Price
12—Rectal	—Insulated.....	<i>Bazin</i>	\$1.60
13—Vaginal	—Insulated.....	<i>Beat</i>	1.85
14—Nasal	—Insulated.....	<i>Bed</i>	1.60
15—Post Nasal	—Insulated.....	<i>Beef</i>	2.10
16—Urethral	—Insulated.....	<i>Bela</i>	1.60
17—Inner Ear	—Insulated.....	<i>Belt</i>	1.60
18—Tongue	—Insulated.....	<i>Benzol</i>	2.00
21—Ozone Generator, only.....		<i>Bidet</i>	7.50
22—Ozone Generator, complete.....		<i>Bidwy</i>	10.00
23—Special Heavy Glass Urethral.....		<i>Gull</i>	1.00
24—Special Heavy Glass Throat.....		<i>Gum</i>	.75
36—Insulated Prostatic Electrode.....		<i>Inpros</i>	2.50
37—Adenoid Electrode—Insulated (Murray).....		<i>Maner</i>	2.50
049—Insulated Rubber Handle and Cord (For 1/2" Tubes).....		<i>Blind</i>	3.30
49—Insulated Rubber Handle and Cord (For 5/8" Tubes).....		<i>Block</i>	6.00
61—Throat (Heavy Glass).....		<i>Breath</i>	1.00
061—Dental Pyorrhea, 1/2" (Heavy Glass).....		<i>Brein</i>	1.00
062—Dental Cocain, 1/2" (Heavy Glass).....		<i>Bridge</i>	1.00
063—Dental Cavity, 1/2" (Heavy Glass).....		<i>Bridle</i>	1.00
064—Dental Outer Gum, 1/2" (Heavy Glass).....		<i>Brim</i>	1.00

Insulated Shock Proof Handle for High Frequency Electrodes

Made entirely of one piece of hard rubber, with the heavy insulated connecting cord fastened securely to the spring brass clamp inside.


No.	Code	Price
049—For 1/2" Electrodes.....	<i>Blind</i>	\$3.30
49—For 5/8" Electrodes.....	<i>Block</i>	6.00



No. 80

No.	Code	Price
80—Extra Long Protected Handle.....	<i>Blesp</i>	\$10.00

Non-vacuum High Frequency Electrodes

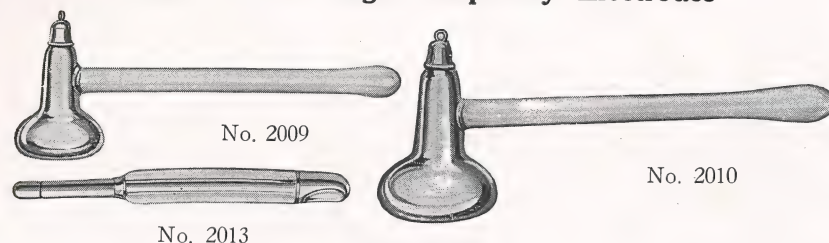

The Silvered "Non-vacuum" Tubes are made in the same sizes and designs as the regular cataloged Vacuum Electrodes described in the foregoing. Plain or Insulated will be furnished, as ordered.

No.	Description	Code	Price
2001—Surface	—Plain—2-inch face	<i>Rabat</i>	\$5.00
2002—Rectal	—Plain	<i>Rabid</i>	5.00
2003—Vaginal	—Plain	<i>Racer</i>	5.00
2004—Nasal	—Plain	<i>Raket</i>	5.00
2005—Throat	—Plain	<i>Radle</i>	5.00
2006—Urethral	—Plain	<i>Radio</i>	5.00
2007—Eye	—Single	<i>Radex</i>	5.00
2008—Eye	—Double	<i>Raflo</i>	5.00
2009—Surface	—Condenser Type, Medium	<i>Raged</i>	5.00
2010—Surface	—Condenser Type, Large	<i>Rally</i>	5.00
2011—Comb	—Scalp	<i>Ramie</i>	5.00
2012—Rectal	—Insulated	<i>Ranch</i>	5.00
2013—Vaginal	—Insulated	<i>Randy</i>	5.00
2014—Nasal	—Insulated	<i>Range</i>	5.00
2015—Post Nasal	—Insulated	<i>Rapid</i>	5.00
2016—Urethral	—Insulated	<i>Rasal</i>	5.00
2017—Inner Ear	—Insulated	<i>Ratan</i>	5.00
2018—Tongue	—Insulated	<i>Ravel</i>	5.00
2023—Urethral	—Special Heavy Glass	<i>Razee</i>	5.00
2024—Throat	—Special Heavy Glass	<i>Razor</i>	5.00
2025—Cataphoresis		<i>Reach</i>	5.00
2030—Corn	—Small Depression	<i>Rebec</i>	5.00
2033—Outer Throat		<i>Rebus</i>	5.00
2034—Spinal		<i>Recal</i>	5.00
2036—Prostatic	—Insulated	<i>Recto</i>	5.00
2061—Dental Pyorrhea	—Heavy Glass	<i>Refit</i>	5.00
2062—Dental Cocain	—Heavy Glass	<i>Reign</i>	5.00
2063—Dental Cavity	—Heavy Glass	<i>Reims</i>	5.00
2064—Dental Outer Gum	—Heavy Glass	<i>Relax</i>	5.00

These Electrodes, with exception of Nos. 2009, 2010, and 2025 will have our regular $\frac{5}{8}$ " shanks.

Nos. 2009, 2010 and 2025 have Insulated Handles blown on the electrodes themselves.

Non-Vacuum Tubes may be had to fit the $\frac{1}{2}$ " Handles by placing "O" before catalog number when ordering, except those which have handles attached.


Mercury Quartz High Frequency Electrodes

A considerable amount of ultra-violet radiation is emitted in addition to the effect of the usual vacuum high frequency discharge.

No.	Description	Code	Price
2090	Mercury Quartz H. F. Electrode (Pointed Urethral)	<i>Afar</i>	\$25.00
2091	Mercury Quartz H. F. Electrode (Ins. Inner Ear)	<i>Afix</i>	25.00
2092	Mercury Quartz H. F. Electrode (Dental)	<i>Aged</i>	25.00
2093	Mercury Quartz H. F. Electrode (Outer Gum)	<i>Agni</i>	25.00
2094	Mercury Quartz H. F. Electrode (Surface—flat)	<i>Agog</i>	32.00
2095	Mercury Quartz H. F. Electrode (Ins. Vaginal)	<i>Ainu</i>	32.00
2096	Mercury Quartz H. F. Electrode (Ins. Rectal)	<i>Ahab</i>	32.00
2097	Mercury Quartz H. F. Electrode (Pointed Orificial)	<i>Ahem</i>	32.00

Universal Handle for High Frequency Electrodes

Insulated section made of hard pressed fiber, having nickel-plated brass spring clamp on end for holding Electrodes firmly in position. Large swivel ring connector to which is hooked the insulated cord, permits of perfect freedom of movement. Made in two sizes.



No.	Description	Code	Price
050	For $\frac{1}{2}$ " Electrodes	<i>Boldo</i>	\$1.30
50	For $\frac{5}{8}$ " Electrodes	<i>Bolus</i>	1.30

Adjustable High Frequency Handle




Nickel-plated clamp on end of long fibre insulated handle is arranged to swivel freely as desired to any angle. A very convenient arrangement especially for orificial work.

No.	Description	Code	Price
56		<i>Roman</i>	\$1.65

Nagelschmidt Condensation Electrodes

Suggested by Dr. Franz Nagelschmidt. Made of very heavy glass, filled with metal in powdered form.

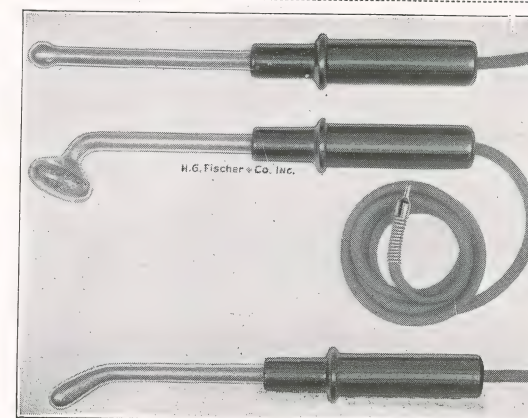

No.	Description	Code	Price
95	Nagelschmidt filled glass electrode, with ball-shaped end	<i>Withal</i>	\$9.00
96	Nagelschmidt filled glass electrode, with flat surface	<i>Wither</i>	9.00
97	Nagelschmidt filled glass electrode, with angular end	<i>Withie</i>	9.00



Insulated High Frequency Cord

This cord is made of a stranded copper conductor, covered with several layers of pure gum rubber, cotton covered. At one end is mounted our standard cord tip ($\frac{1}{8}$ inch), which will fit any of our machines, and on the other end is mounted a swivel clasp. Cord is very flexible.

No.		Code	Price
51	Heavy Cord 4' long.....	Gait	\$1.70
51-5	Heavy Cord, 5' long.....	Hirtz	1.90
51-6	Heavy Cord, 6' long.....	Hoche	2.00
51-7	Heavy Cord, 7' long.....	Hodge	2.10

Extra cable, 15c foot

Extra Heavy Insulated Cable


Made similar to our No. 51 but with very heavy rubber insulation.

No.		Code	Price
83	Extra Heavy Protected High Frequency Cord, 5' long.....	Malle	\$3.00

Heavy High Frequency Cord

No.		Code	Price
85	Heavy High Frequency Cord, with special tip for Type "V" Outfit (5-foot)	Wailfu	\$3.15

Fulguration Electrode

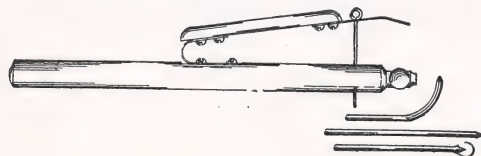

Fulguration is the best known method of applying the High Frequency Current for the removal of warts, moles and similar growths.

No.		Code	Price
20	Fulguration Electrode and three tips.....	Gadol	\$2.70

Fulguration Wire

Steel music wire, covered with pure gum rubber, for introduction through the cystoscope. When used in connection with one of our High Frequency machines excellent results may be obtained in the removal of growths in the urinary bladder.

No.		Code	Price, Foot
40	Fulguration Wire	Gag	\$0.10

Fischer Bladder Fulguration Electrode



A special fulguration electrode for use in the bladder through a cystoscope. Made of a hard wire center, insulated with a very small oiled silk covering. Has solid silver tip, olive shaped, of 2mm. diameter and about 4mm. long. Other end is arranged to accommodate an ordinary cord tip.


No.		Code	Price
41	Complete as illustrated.....	Gagtip	\$1.90

Special Tonsil Fulguration Electrode




No.		Code	Price
29	Special Throat Fulguration Electrode similar to our No. 23 with wire tip mounted in end.....	Gerdy	\$1.50

Improved Ear Electrode

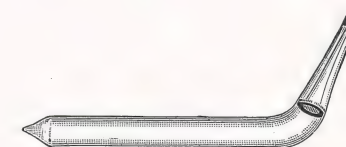

Properly shaped, and well insulated.

No.		Code	Price
43		Gabell	\$1.60


Glass Vacuum Handle

For indirect treating with the High Frequency Current.

No.	Code	Price
53 Glass Handle	<i>Bismal</i>	\$1.75

Indirect Treatment Handles

No.	Code	Price
54 Similar to No. 53, except that it is arranged to fit No. 49 Shock Proof Handle. For Indirect Treating	<i>Banter</i>	\$0.65
054 Same as No. 54, but made to fit the 049 Handle.....	<i>Bantam</i>	.65

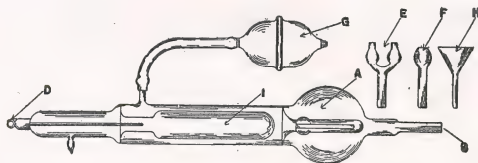Ozone Generator

No. 22

An ALL GLASS Ozonizer, made in one piece. Has two compartments, one for holding the purifying oils, and a vacuum chamber to which is connected the wire from any high frequency source.

No.	Code	Price
22 Ozone Generator, complete as illustrated, with oils	<i>Bidwy</i>	\$10.00
70 Rubber Bulb, only.....	<i>Ozbule</i>	.50
71 Hose Connection—foot	<i>Ozhoco</i>	.10
72 Mouth Piece	<i>Ozmopi</i>	.20
73 Nose Piece	<i>Oznose</i>	.50
74 Funnel	<i>Ozfunl</i>	.40
75 1 oz. Bottle Pine Needle Oil.....	<i>Malmo</i>	.75
76 1 oz. Bottle Eucalyptus Oil.....	<i>Malta</i>	.40

Cord Tip Adapters

To enable operators to use cords with 3/32 inch tips with apparatus having 5/32 inch binding post or attachment openings, or vice-versa.



No. 1335

No.	Code	Price
1335 Increases size of 3/32" tip to 5/32".....	<i>Corter</i>	\$0.30
1336 Decreases size of 5/32" tip to 3/32".....	<i>Adacor</i>	.30


Eye Magnet

Constructed to operate from any low voltage source, up to 10 volts.

No.	Code	Price
1568 Eye Magnet	<i>Acoon</i>	\$5.50

Diagnostic Illuminator and Shield

Consisting of a long metal holder, with a green silk covered connecting cord, and a specially designed opal bulb with a lens blown in the end. This focuses an intense light to the area desired.

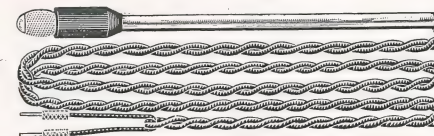

No. 321



No. 322




No. 324


No.	Code	Price
321 Illuminator, complete with Tungsten lamp.....	<i>Analog</i>	\$3.25
322 Extra Tungsten bulb.....	<i>Acid</i>	1.00
324 Polished Nickel-plated Shield for No. 321.....	<i>Agile</i>	.55

Note: When ordering these cords for the Fischer Senior "FO," "LO," "G" or "GP" Diathermy Outfits, specify No. "321G" which are supplied with special tips.

Tongue Depressor and Diagnostic Illuminator



Cat.
No.
340

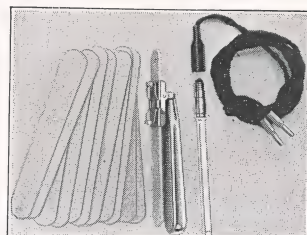


Consisting of an aluminum handle with folding end-piece through which are slipped ordinary wooden tongue strips, twelve wooden blades, green silk connecting cord, lamp socket and opal lamp.

The special opal lamp is supported in spring clips above the wooden tongue blades, and is easily removed. This lamp throws an intense white light, properly focused.

No.		Code	Price
335	Diagnostic Illuminator, with Cords and Socket, and Opal Lamp	<i>Usurp</i>	\$4.75
336	Special Diagnostic Lamp Bulb, only.....	<i>Uther</i>	3.00
337	Tongue Depressor, only, with twelve blades.....	<i>Uvula</i>	2.50
338	Extra Wooden Tongue Blades, box of 12.....	<i>Vacat</i>	.15
340	Complete Lamp and Tongue Depressor arrangement, including Illuminator with Cords, Holder, and Opal Lamp, Tongue Depressor and 12 Wooden Tongue Blades.....	<i>Vague</i>	7.25

New Fischer Cautery Cords

Flexible copper stranded wire, covered with pure gum rubber, replacing the former cords which were covered with mercerized webbing. May be washed and always kept clean as when new.



No.		Code	Price
1330	6 ft. pair.....	<i>Negro</i>	\$2.75

Note: When ordering these cords for the Fischer Senior "FO," "LO," "G" or "GP" Diathermy Outfits, specify No. 1331, which are supplied with special tips.

Cautery and Diagnostic Transformer




No. 471

The Fischer Cautery and Diagnostic Light Transformer is a compact, neat generator of the closed-core type, consuming very little energy, yet having sufficient output to heat most any Cautery knife on the market. Has a diagnostic lamp circuit with a range of from 1/2 to 12 volts. Can be used with perfect safety for lighting your smallest Cystoscope bulbs, or for illuminating a 12-volt lamp if necessary. Both circuits are perfectly regulated, and durably wound. Case is covered with black leatherette. Contact buttons, regulating levers, and binding posts are of brass, heavily nickel-plated, and mounted on white marble.

No.		Code	Price
470	Transformer only, in carrying case, with connecting cord and attachment plug, for 110 volt, 60 cycle, alternating current.....	<i>Abac</i>	\$27.50
471	Outfit with pair No. 306 Heavy Cautery Cords, 1 No. 305A Cautery Knife, 1 No. 305C Cautery Knife, 1 No. 301 Cautery Handle, 1 No. 321 Diagnostic Illuminator, complete.....	<i>Abaca</i>	33.00

Cautery Knives

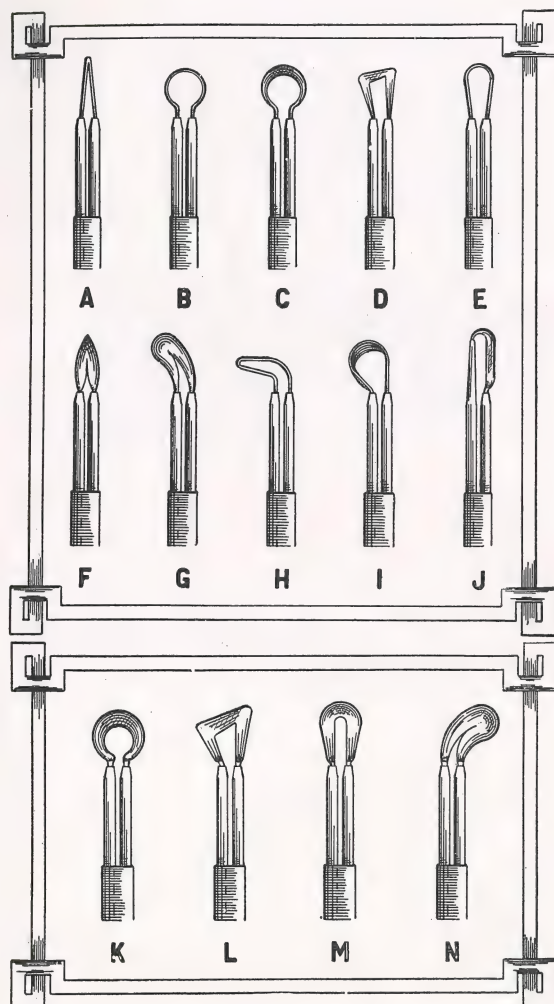


No.	Price
305A to 305J.....	Each, \$0.60
305K to 305N Heavy.....	" .80

Codes *Acmea, Acmeb, Acmec*, etc.

Cautery Knives

The carefully shaped knives are securely mounted into the copper bars. These knives are shaped to conform with most any requirements for all purposes. The copper bars are bound together by a special twisting process, and enameled to withstand heating and handling indefinitely. Knives are made of a special alloy, of high electrical resistance. (See page 48.)

Heavy Cautery Knives and Handle

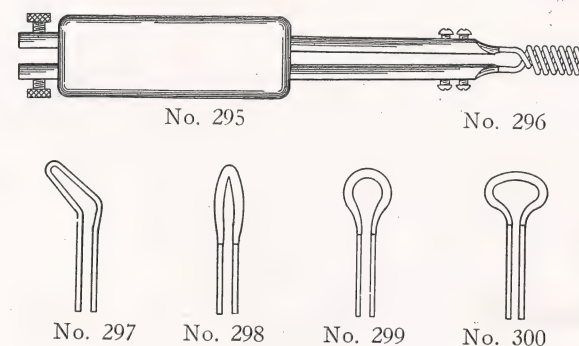

No.		Code	Price
295	Heavy Cautery Handle.....	<i>Pacero</i>	\$12.25
296	Heavy Spiral Cautery Knife.....	<i>Pachan</i>	1.60
297	Heavy Angular Cautery Knife.....	<i>Pacify</i>	2.05
298	Heavy Pointed Cautery Knife.....	<i>Packor</i>	1.30
299	Heavy Plain Loop Cautery Knife.....	<i>Pacton</i>	1.40
300	Heavy Flat Loop Cautery Knife.....	<i>Paddle</i>	1.75


Cautery Handle




Made of a practically indestructible material. Arranged to hold the knives in any one of five positions. Has contact switch for convenience in operating.

No.		Code	Price
301	Cautery Handle	<i>Acetyl</i>	\$2.75

Rotary Converters

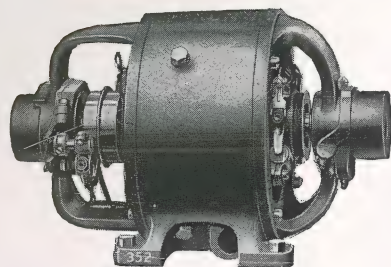

No. 952



No. 950

When direct current, only, is available it is necessary to install a rotary converter to operate any efficient High Frequency machine, or any of the late types of small X-ray Outfits. (The larger X-ray machines contain their own rotary converters.)

Our 110 volt rotaries have a special booster winding which insures a full 110 volt A. C. when operated on 110 volts D. C.



Our 220 volt rotaries are tapped at the proper point to give 110 volts A. C. when operated on 220 volts D. C. This eliminates the use of separate step-up or step-down transformers and the loss of efficiency attending their use.

All our Rotary Converters are equipped with a special Condenser, for line protection.


No.	Code	Price
950 300 Watt capacity—operating on 110 volts D. C., and delivering 110 volts 60 cy. A. C. Designed for our types "C" and "K" and "D" outfits.....	<i>Emolo</i>	\$70.00
952 1000 Watt capacity—operating on 110 volts D. C. and delivering 110 volts 60 cy. A. C. Designed for our Type "L," "Military" and Style "F" Cabinets, also the No. 1, De Luxe or Type "R" X-ray Machines, including enclosed type Starting Box "Scurvy".....	<i>Ennui</i>	175.00
954 500 Watt capacity—operating on 110 volts D. C., and delivering 110 volts 60 cy. A. C. Designed for our Type "G" Diathermy Outfits.....	<i>Enporg</i>	85.00
955 300 Watt capacity—operating on 220 volts D. C., and delivering 110 volts 60 cy. A. C. (See No. 950)	<i>Epul</i>	70.00

No.	Code	Price
957 1000 Watt capacity—operating on 220 volts D. C., and delivering 110 volts 60 cy. A. C. (See No. 952) including enclosed type Starting Box "Seance"	<i>Enter</i>	\$175.00
958 5000 Watt capacity—operating on 220 volts D. C., and delivering 110 volts 60 cy. A. C. Designed for use with Type "S" X-ray Apparatus, including enclosed type Starting Box "Secede"	<i>Encabs</i>	350.00
959 500 Watt capacity—operating on 220 volts D. C., and delivering 110 volts 60 cy. A. C. (See No. 954)	<i>Enpogs</i>	85.00
977 1500 Watt capacity—operating on 110 volts D. C. and delivering 110 volts 60 cy. A. C., including enclosed type Starting Box "Scurvy"	<i>Mutcho</i>	195.00
978 1500 Watt capacity—operating on 220 volts D. C., and delivering 110 volts 60 cy. A. C., including enclosed type Starting Box "Seance"	<i>Myomoa</i>	195.00
2120 2000 Watt capacity—operating on 110 volts D. C. and delivering 110 volts 60 cy. A. C. Designed for our Model "V" Senior Diathermy Cabinet	<i>Yello</i>	220.00
2122 2000 Watt capacity—operating on 220 volts D. C. and delivering 110 volts 60 cycles A. C. Designed for our Model "V" Senior Diathermy Cabinet	<i>Yesty</i>	210.00

Starting Boxes for Rotary Converter




No.	Code	Price
915 Starting Box for 110 V. Rotary 1000 and 1500W..	<i>Scurvy</i>	\$15.00
916 Starting Box for 220 V. Rotary 1000 and 1500W..	<i>Seance</i>	15.00
918 Starting Box for 220 V. Rotary 5000W.....	<i>Secede</i>	21.00

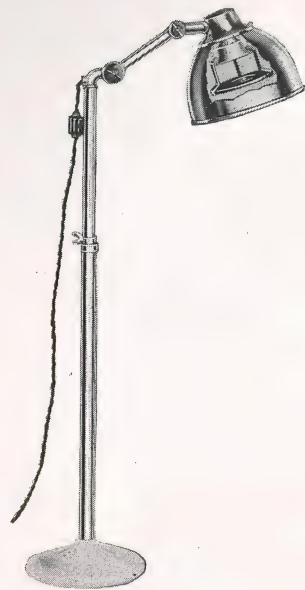

No.		Code	Price
2167	Stand Radiant Lamp.....	<i>Yowli</i>	\$25.00
2169	Stand Infra Red Lamp	<i>Young</i>	27.50
2171	Stand Combination Radiant and Infra Red Lamp	<i>Yugas</i>	29.75

Can be raised to any desirable height and placed in any position, free from "sag" or "let-down." Position is maintained by large nickel plated wing nuts.

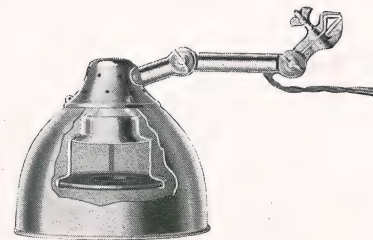


No.		Code	Price
2161	Clamp Radiant Lamp.....	<i>Yucca</i>	\$12.50
2163	Clamp Infra Red Lamp.....	<i>Yuman</i>	15.00
2165	Clamp Combination Lamp.....	<i>Yuita</i>	17.25

Both the Stand and Clamp Lamp are supplied in three styles:

1. With a 260 Watt Carbon Bulb.
2. With Indestructible Infra Red Generator.
3. Combination of the Carbon Bulb and the Infra Red Generator.

In ordering, be sure to specify style desired.


Indestructible Infra Red Generator

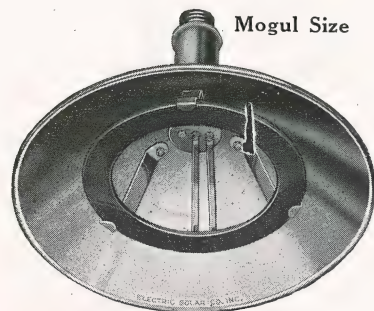

Mogul Size


No.		Code	Price
2173	Infra-red Generator, with polished reflector, to use in place of 1,000 or 1,500 watt bulb	<i>Yulet</i>	\$25.00
2174	Infra-red Generator, same as illustrated and described under catalog No. 2173, but without reflector	<i>Yulno</i>	22.50
2175	Infra-red Generator of 500 watt capacity, as used with stand and clamp lamps illustrated above	<i>Yuigr</i>	5.00

Fischer "Radiolite"

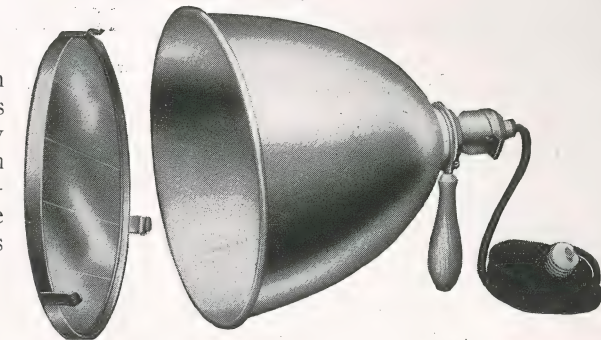

The reflector on the "Radiolite" is made of highly polished aluminum spun to true parabolic shape. The outside diameter is ten inches.

No.		Code	Price
154	Fischer "Radiolite," 10" Reflector Light Globe, Connecting Cord and Plug, no screen.....	<i>Hamul</i>	\$12.00

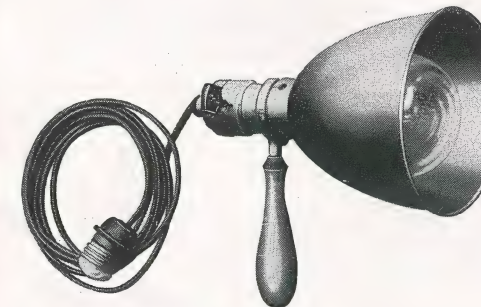

Fischer "Radiolite Junior"

Made of same material and same style as the larger lamp above, but of five-inch diameter only.

No.		Code	Price
152	5" Reflector with Lamp, Connecting Cord and plug	<i>Hack</i>	\$7.00

Bulbs for Therapeutic Lamps


No.		Code	Price
168	Extra Bulb for 10" Lamp, 375 Watt	<i>Hegar</i>	\$3.70
166	Extra Bulb for 5" Lamp, 128 Watt	<i>Hectic</i>	1.75
181	1000-watt clear bulb	<i>Udder</i>	6.00
183	1500-watt clear bulb	<i>Uhase</i>	8.00
182	1000-watt blue "daylight" bulb	<i>Ugric</i>	9.50
184	1500-watt blue "daylight" bulb	<i>Uhlan</i>	10.00

Price List of Therapeutic Carbons

November 21, 1928.


Effective this date the following prices will be in effect on Carbons:

Cat. No.	Type of Carbon	Lots of 25	Lots of 50	Lots of 100
2177	("A") 8mm. x 6"	\$2.53	\$5.06	\$9.20
2178	("C") 8mm. x 6"	3.44	6.88	12.50
2179	("D") 8mm. x 6"	2.25	4.50	8.20
2180	("E") 8mm. x 6"	3.02	6.05	11.00
2181	("G") 8mm. x 6"	3.25	6.50	11.80
2182	("H") 8mm. x 6"	2.42	4.84	8.80
2183	("B") 8mm. x 6"	2.48	4.95	9.00
2184	("F") 8mm. x 6"	5.36	10.72	19.50
2185	("K") 8mm. x 6"	6.68	13.36	24.30
2188	("A") 8mm. x 12"	4.13	8.25	15.00
2189	("C") 8mm. x 12"	5.78	11.55	21.00
2190	("D") 8mm. x 12"	3.25	6.49	11.80
2191	("E") 8mm. x 12"	4.68	9.35	17.00
2192	("G") 8mm. x 12"	5.50	11.00	20.00
2193	("H") 8mm. x 12"	3.71	7.42	13.50
2194	("B") 8mm. x 12"	3.90	7.81	14.20
2195	("F") 8mm. x 12"	9.82	19.64	35.70
2196	("K") 8mm. x 12"	12.48	25.02	45.50

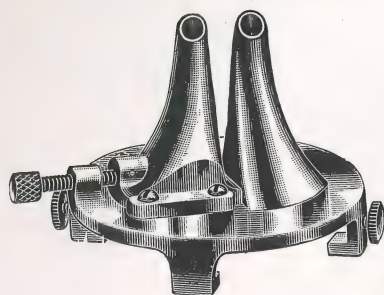Hollender-Cottle Bilateral Nasal Speculum**for Intranasal Ultra-Violet Irradiation
without the Use of Quartz Rods**

The new "H-C" Bilateral Nasal Speculum offers an improved method for irradiating the nasal mucosa with ultra-violet light. It has several distinct advantages. The raying is direct. It is time saving. It may be used in conjunction with quartz rod irradiation, the latter serving best for posterior nasal work. The speculum is easily attached to a Kromayer Lamp. The adjustments make it possible to treat any nose.

No.	Code	Price
1488	Vulcan	\$15.00

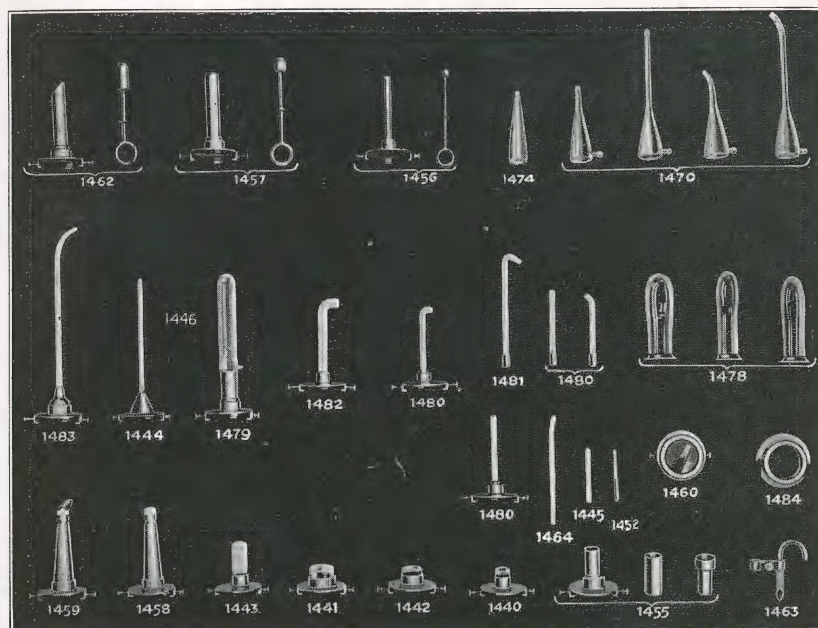Applicators and Spare Parts


In local conditions of skin or cavity, the range of application of the Kromayer or Alpine Sun lamps depends upon the variety of applicators available. In the selection one should be governed by the extent of work in which the lamp is to be used.

These applicators are made of the best grade of clear quartz which insures the greatest possible transmission of Ultra-violet rays.

[NOTE For Quartz Ultra-violet Burners
and Burner Repairs, see page 77]

No.		Code	Price
1440	Quartz Lens Applicator Rod (Small).....	Mirth	\$20.00
1441	Quartz Lens Applicator Square.....	Mirza	27.00
1442	Quartz Lens Applicator Rod (Medium).....	Misty	23.00
1443	Hemorrhoid Applicator.....	Miter	36.00
1444	Holder for Quartz Rods.....	Mocha	7.50
1445	Quartz Rod Straight End 2 3/4" long.....	Modes	12.00
1446	Quartz Rod Shaped End 6 3/4" long.....	Modoc	24.00
1447	Blue Ultra-violet Glass 2mm.....	Moera	6.00
1448	Blue Ultra-violet Glass 3mm.....	Mogul	6.00
1449	Blue Ultra-violet Glass 4mm.....	Mohur	6.00
1450	Blue Ultra-violet Glass 5mm.....	Moire	6.00
1451	Mica Protection Window.....	Molar	1.00
1452	Weaver Applicator.....	Molli	13.50
1453	Rubber Tubing, Foot.....	Moult	.30
1454	Quartz Window.....	Monus	6.50
1455	Sharpe Localizer and 3 Tubes.....	Monad	7.00
1456	McManus Sinus Applicator.....	Mongo	7.50
1457	Plank Proctoscope.....	Monke	9.75
1458	Plank Pharyngeal Applicator.....	Monot	19.00
1459	Baldwin Laryngoscope.....	Mooch	32.00
1460	Blue Window, Complete.....	Moody	10.50
1461	Blue Window, Less Holder.....	Moose	6.50
1462	Burrow's Prostatic Applicator.....	Mopey	10.50
1463	Rubber Tube Clamp.....	Moral	1.25
1464	Mehler Nasal Applicator.....	Morin	24.00
1465	Protection Goggles.....	Mossy	.40
1466	Ladabeck Quartz Irrigator (Small).....	Motif	22.50
1467	Ladabeck Quartz Irrigator (Medium).....	Motto	22.50
1468	Ladabeck Quartz Irrigator (Large).....	Mound	29.00
1469	Ladabeck Quartz Irrigator (Extra Large).....	Mourn	29.00
1470	Ladabeck Quartz Irrigator (Set of 4).....	Movie	103.00
1471	Daly Pyorrhea Applicator (Set of 3).....	Mower	45.00
1472	Bainbridge-Lippman Applicator.....	Mucky	18.00
1474	Mayer Aural Applicator.....	Mufin	15.00
1475	Wagner Quartz Speculum (Size A).....	Muggy	24.00
1476	Wagner Quartz Speculum (Size B).....	Mulct	30.00
1477	Wagner Quartz Speculum (Size C).....	Muley	36.00
1478	Wagner Quartz Speculum (Set of 3).....	Mumbl	90.00
1479	McCaskey's Prostatic Applicator.....	Mumps	36.00
1480	Sampson Pyorrhea Applicator (Set of 3).....	Mungo	32.50
1481	Sampson Hay Fever Applicator.....	Mural	24.00
1482	Sampson Laryngoscope.....	Usage	38.00
1483	Quartz Urethral Applicator.....	Usbek	32.00
1484	Alpine Kromayer Applicator Adapter, to attach Quartz applicators to the Alpine Lamp—Fur- nished free of charge.....	Usher	
1486	Ashland Universal Pyorrhea Applicator.....	Varixx	26.50

ULTRA-VIOLET TOLERANCE GAUGE

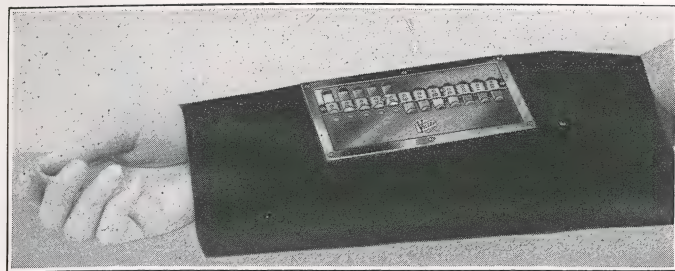


A practical device for determining individual tolerance to ultra-violet radiation. The protective skirt, as illustrated, is part of the device.

No.	Code	Price
U. V. Tolerance Gauge.....	<i>Uvgage</i>	\$2.50

Condenser (Static Arrester)

Used in connection with powerful High Frequency apparatus for protection to line. Mounted on a slate slab, in a metal box.

No.	Code	Price
960 Condenser for A. C. lines..	<i>Tetort</i>	\$15.25
961 Condenser for D. C. lines as used across Rotary Converters	<i>Recopo</i>	10.00

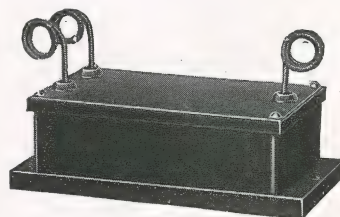

Pilot Lamp

An indicating lamp bulb used on most of our Portable and Cabinet Apparatus.

No.	Code	Price
325 Plain Bulb	<i>Larrup</i>	\$0.40
326 Ruby Bulb	<i>Lodge</i>	.40




Casters

1260	4 3/4" wheel with 5/8" rubber face	<i>Cascar</i>	\$2.50
1261	2 1/2" wheel with 1 1/16" felt face	<i>Castye</i>	1.80
1262	2" wheel with 1" fibre face....	<i>Casfos</i>	.90
1263	1 5/8" wheel with 3/4" fibre face	<i>Casmal</i>	.45
1264	2 3/4" wheel with 1/2" rubber face	<i>Virtue</i>	1.50
1265	2" wheel with 3/4" rubber face	<i>Visage</i>	1.00

Pneumatic Air Hammer Vibrator

Finished in black enamel and nickel-plate. Arranged to screw on end of pressure handle, or if desired will be furnished complete with a hard rubber handle and pressure hose to attach to any source of compressed air. Degree of vibration controlled by air valve in handle.

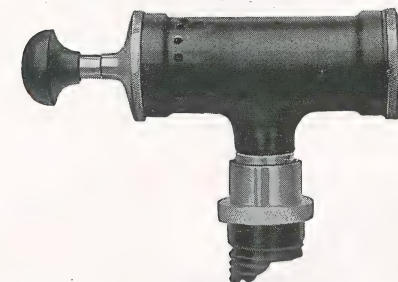

No. 1510



No. 1512



No. 1511




No. 1513



No. 1514

No.	Code	Price
1510 Air Hammer Vibrator.....	<i>Canker</i>	\$14.00
1511 Ball Applicator for No. 1510.....	<i>Canon</i>	.95
1512 Spine Applicator for No. 1510.....	<i>Canula</i>	1.75
1513 Curved Applicator for No. 1510.....	<i>Capul</i>	1.30
1514 Large Body Applicator for No. 1510.....	<i>Caput</i>	1.10

Dr. Pope's Dilators

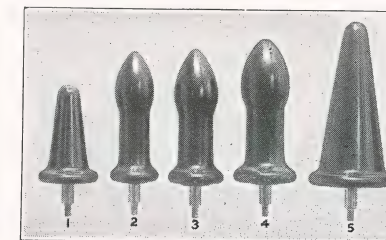

No.	Code	Price
1340 No. 1 size Dilator.....	<i>Popone</i>	\$1.75
1341 No. 2 size Dilator.....	<i>Poptwo</i>	1.75
1342 No. 3 size Dilator.....	<i>Poptre</i>	1.75
1343 No. 4 size Dilator.....	<i>Popfor</i>	1.75
1344 No. 5 size Dilator.....	<i>Popfir</i>	1.75
1345 Set of five Dilators.....	<i>Popset</i>	8.50

Cavity Vibratodes



No. 1560



No. 1560A



No. 1561



No. 1561A




No. 1562



No. 1562A

No.		Code	Price
1560	Vaginal Vibratode, Hard Rubber.....	<i>Kane</i>	\$0.60
1560A	Vaginal Vibratode, Soft Rubber Cap.....	<i>Kaolin</i>	.35
1561	Rectal Vibratode, Hard Rubber.....	<i>Karma</i>	.60
1561A	Rectal Vibratode, Soft Rubber Cap.....	<i>Karoo</i>	.15
1562	Flexible Rubber Colon Catheter.....	<i>Kauri</i>	1.00
1562A	Dilating Bag for No. 1562 Catheter.....	<i>Keany</i>	.50

Pennington Rectal Cone

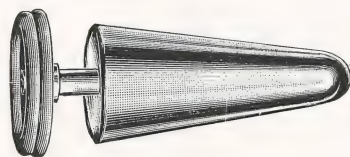


The Pennington Rectal Cone adapted for use with the No. 1551 Vibratode as furnished with Fischer cabinets having the motor and pump features.

No.		Code	Price
1590	Including Metal Holder.....	<i>Penco</i>	\$5.00

Pneumatic Rubber Vibratodes



No. 1550




No. 1550R



No. 1551R



No. 1551

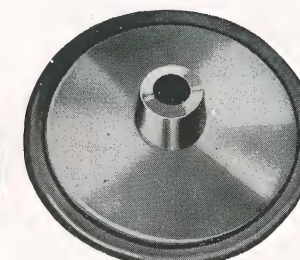


No. 1552



No. 1552R

No.		Code	Price
1550	Small Size Vibratode, Rubber Holder.....	<i>Kation</i>	\$0.30
1550R	Small Size Vibratode, Rubber Cap.....	<i>Kabul</i>	.25
1551	Medium Size Vibratode, Metal Holder.....	<i>Kadesh</i>	.90
1551R	Medium Size Vibratode, Rubber Cap.....	<i>Kaffir</i>	.30
1552	Large Size Vibratode, Metal Holder.....	<i>Kago</i>	1.10
1552R	Large Size Vibratode, Rubber Cap.....	<i>Karek</i>	.30

Special Ear Vibratode (Owen)



An ingenious device for the application of vibration and variable sound tones simultaneously. Must be tried to be appreciated.

No.		Code	Price
1567		<i>Souvib</i>	\$1.50

Sinus Suction Tube

So constructed that it is impossible for the aspirated matter to enter the second bulb or tubing. Furnished with 4 ft. rubber tubing and a metal attachment to fit the Vacuum Handle supplied with our Cabinet Apparatus.

No.	Code	Price
1503	<i>Jesitu</i>	\$2.00

Pressure Handle

Hard Rubber Handle, fitted with control valve, for use with Vibrator No. 1510 if you have no T. & P. Cabinet.

No.	Code	Price
1516	<i>Cyprus</i>	\$7.40

Pressure Tubing

Extra Pressure and Vacuum Tubing, cotton covered any lengths.

No.	Code	Price
1517	<i>Cyanic</i>	Foot, \$0.25




No. 1517

De Vilbiss-Fischer Connector

Arranged to fit the tapered end of the pressure handle furnished with Fischer Cabinets, and to accommodate the regular De Vilbiss bottles.

No.	Code	Price
1530 Metal Connector	<i>Karyon</i>	\$0.40

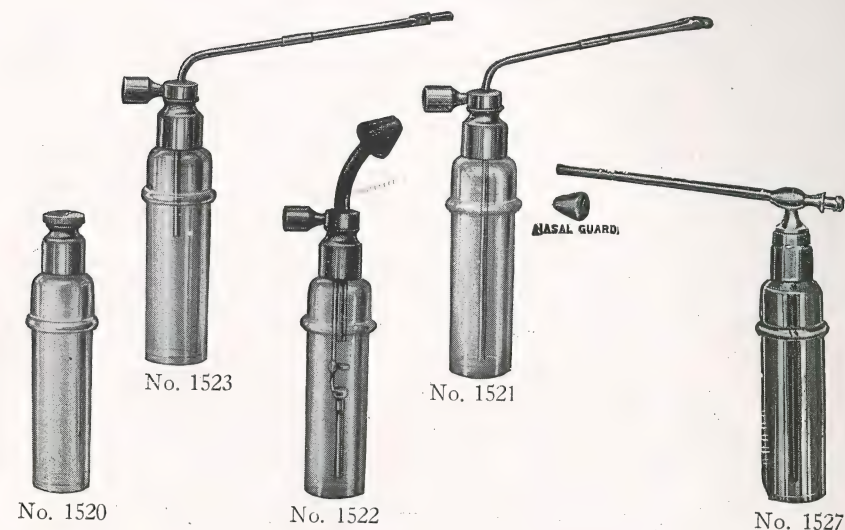
De Vilbiss Atomers


No.	Code	Price
1520 Empty bottle only, with stopper.....	<i>Kali</i>	\$0.30
1521 Atomer. Sprays any liquid, oil or aqueous, in any direction desired	<i>Kalium</i>	1.60
1522 Nebulizer. Produces a vapor; for oils only. The vapor can be weakened by turning the little table to a horizontal position, or strengthened by turning it to a perpendicular position	<i>Kamala</i>	1.60
1523 Powder Blower. Diffuses powder perfectly in any direction	<i>Kalot</i>	1.60
1527 Atomer. For spraying oils and aqueous solutions. It can be easily cleaned by unscrewing the heel-piece and wiping the tube.....	<i>Kilter</i>	1.60

Numbers 1521 and 1527 are provided with an extra hard rubber tube for spraying corrosive solutions.


Eustachian Tube Opener

No.	Code	Price
1575 Metal Eustachian Tube Opener.....	<i>Kennel</i>	\$0.50



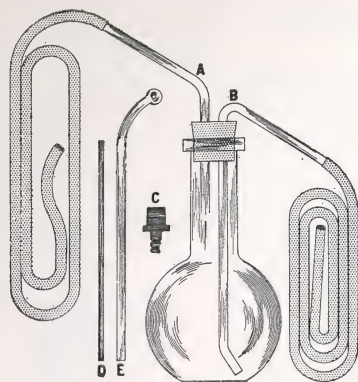Suction Bottle

No.		Code	Price
1577	Suction Bottle, complete as illustrated	<i>Hepar</i>	\$3.50
1532	Extra Bottle only.....	<i>Hatch</i>	1.15
1533	Rubber Hose, ft.....	<i>Hauld</i>	.25
1534	Silver Catheter	<i>Haven</i>	1.00
1535	Glass Syphon	<i>Hawse</i>	.40

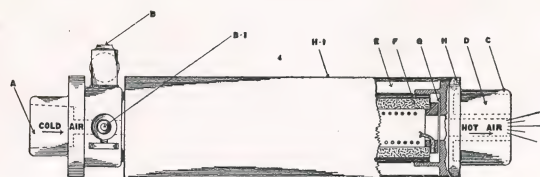
Air Heater

Output is under perfect control as the energy is obtained from the Cautery circuit, and any degree of heat may be maintained indefinitely.

No.		Code	Price
1570	Fischer Air Heater, with extra unit.....	<i>Acoin</i>	\$7.50
1571	Fischer Air Heater Unit.....	<i>Keck</i>	1.00
1572	Air Spreader Attachment.....	<i>Keel</i>	.50

Special Cut-off

Unless otherwise advised, the Cut-off will be furnished with a short length of rubber tubing special metal attachment to fit over the end of our Pressure Handle, as indicated on illustration. Also furnished without special "Y" Valve Attachment for side of cabinet, as indicated on page 63 under No. 1110.

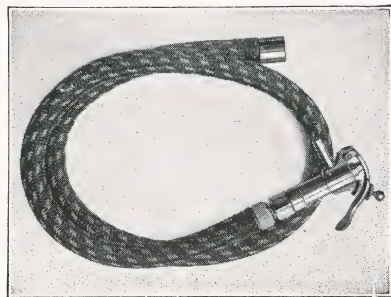

No.		Code	Price
1528	Special Cut off	<i>Kirtle</i>	\$5.00

Pressure Valve Attachment for Fischer Combination Cabinets

No.		Code	Price
1110	Special "Y" Valve with De Vilbiss No. 1528 Cut-off with 6' hose.....	<i>Ictus</i>	\$14.65
1111	Pressure Valve only.....	<i>Igloo</i>	8.20
1517	Extra Pressure Hose.....	<i>Cyanic</i>	Foot, .25

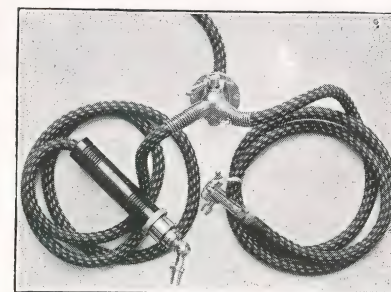


Illustration No. 1

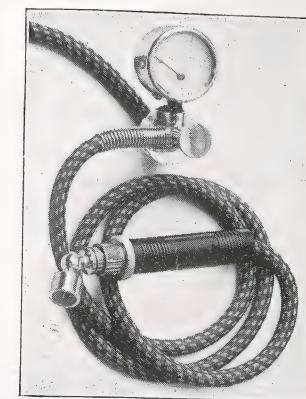


Illustration No. 2

Vacuum Valve Arrangement

The Vacuum Handle and 6-foot tube, illustrated under No. 2 is not included with the regular No. 1113, as these parts are already furnished with each of our cabinets.

The regular Pressure Handle and 6-foot hose as shown in illustration No. 1, above, is not included with the regular No. 1110 Valve order, as these parts are already furnished with each of our cabinets.

No.		Code	Price
1113	Vacuum Gauge and Regulating Valve with 30-inch hose	<i>Ides</i>	\$13.00
1114	Vacuum Gauge only	<i>Idle</i>	3.50
1517	Vacuum Hose.....	<i>Cyanic</i>	Foot, .25


**Exhaust Filter**

For mounting between the cup holder and the vacuum handle proper. Stuffed with absorbent cotton, it prevents the passage of the extracted fluid to the pump.

No.		Code	Price
1504	Exhaust Filter	<i>Jefilt</i>	\$1.75

Glass Exhaust Cups

Made of smoothly finished, plain glass, with rim of heavier glass on the edges. The ends are fitted to the rubber bushing in the vacuum handle on all Fischer cabinets containing pump features.

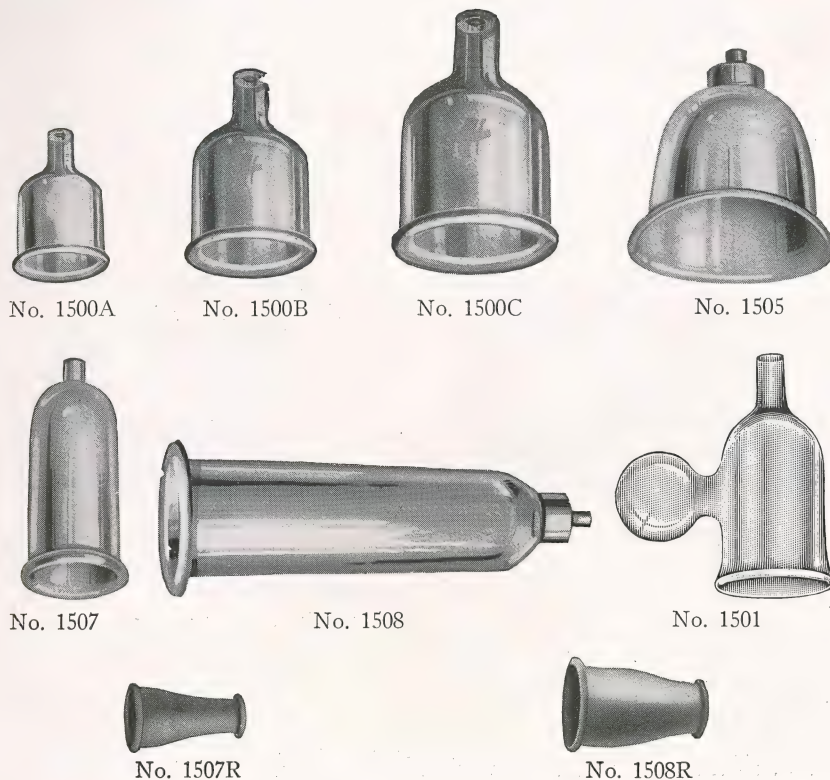


No.		Code	Price
1500A	Vacuum Cup, 1" Diameter.....	<i>Jeloy</i>	\$0.35
1500B	Vacuum Cup, 1½" Diameter.....	<i>Jervin</i>	.40
1500C	Vacuum Cup, 2" Diameter	<i>Jesuit</i>	.40
1501	Exhaust Cup with trap.....	<i>Jesty</i>	.85
1505	Glass Breast Cup.....	<i>Jigger</i>	1.80
1507	Glass Panaris Cup.....	<i>Joint</i>	.80
1507R	Soft Rubber Panaris Casing.....	<i>Jolly</i>	.40
1508	Glass G. U. Tube.....	<i>Joule</i>	1.95
1508R	Soft Rubber G. U. Casing.....	<i>Jugal</i>	.75

**The Fischer-DeVilbiss
Sinus Suction Bottle**

No. 1790 Consisting of bottle, nose piece, 2 silver catheters, rubber tube and connectors. Code, *Umbra*. Price.....\$6.50

No.		Code	Price
1791	Bottle and Nose Piece.....	<i>Unarm</i>	\$1.60
1792	Small Silver Catheter	<i>Unbar</i>	1.30
1793	Large Silver Catheter	<i>Uncle</i>	1.60
1794	Hose and Connectors	<i>Undue</i>	1.50

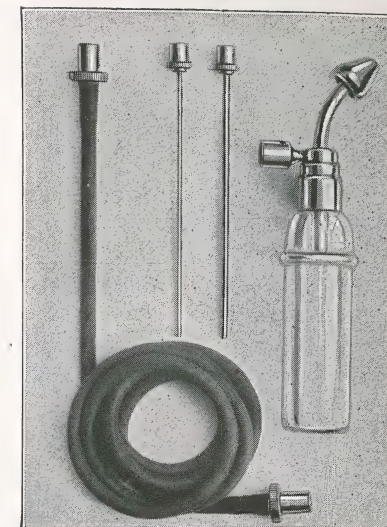**Rubber Vacuum Cups**

No.		Code	Price
1555	Flexible Rubber Vacuum Cup.....	<i>Kale</i>	\$0.45
1556	Flexible Rubber Cup (large).....	<i>Kandy</i>	1.00
1573	Metal Attachment for connecting the rubber cups to the vacuum handle.....	<i>Kelpie</i>	.25

Motor and Pump Grease

No.		Code	Price
1582	Small can	<i>Ketch</i>	\$0.20
1589	½ lb. can.....	<i>Kease</i>	.70

Books on Physiotherapeutic Subjects on Diathermy

No.		Code	Price
1703	"Diathermy in Medical and Surgical Diseases" by Saberton.....	<i>Insabe</i>	\$3.00
1734	"Treatment of Gonococcal Infection by Diathermy" by E. P. Cumberbatch, M.D., and C. A. Robinson, M.D.....	<i>Vulgar</i>	3.75
1737	"Diathermy—Its Production and Uses in Medicine and Surgery" by Elkin P. Cumberbatch, M.D.....	<i>Incumb</i>	6.00
1742	"Diathermy and Its Application to Pneumonia" by Harry Eaton Stewart, M.D.....	<i>Instew</i>	3.00
1746	"Practical Electrotherapeutics and Diathermy" by G. Betton Massey, M.D.....	<i>Verbal</i>	6.50
1747	"Practical Index to Electrophysiotherapy" by J. E. G. Waddington, M.D.....	<i>Verbos</i>	6.50
1750	"Diathermy in the Treatment of Genitourinary Diseases with Especial Reference to Cancer" by Budd C. Corbus, M.D., and Vincent J. O'Connor, M.D.....	<i>Corcon</i>	5.00
1753	"The Practice of Physiotherapy" 1926 edition, by C. M. Sampson, M.D.....	<i>Walrus</i>	10.00
1756	"High Frequency Practice" (Fourth Edition) by Burton Baker Grover, M.D.....	<i>Veaous</i>	6.00
1758	"Physiotherapy Theory and Clinical Application" by Harry Eaton Stewart, M. D.....	<i>Vesica</i>	7.50
1971	"Surgery of Neoplastic Diseases by Electrothermic Methods" by George A. Wyeth, M.D.....	<i>Ahoy</i>	7.50
1975	"Physical Therapy in Diseases of the Eye, Ear, Nose and Throat" by A. R. Hollender, M. D., and M. H. Cottle, M. D.....	<i>Warley</i>	5.00
1976	"Electrothermic Methods in the Treatment of Neoplastic Diseases" by J. Douglas Morgan, M. D.....	<i>Washer</i>	2.50
1978	"Principles of Physiotherapy" by Turrell.....	<i>Wattle</i>	3.85

On High Frequency Currents

1747	"Practical Index to Electrophysiotherapy" by J. E. G. Waddington, M. D.....	<i>Verbos</i>	6.50
1756	"High Frequency Practice" (Fourth Edition) by Burton Baker Grover, M. D.....	<i>Venous</i>	6.00

On Constant Currents

1973	"Galvanic and Low Voltage Wave Currents" by Drs. Massey and Morse	<i>Airy</i>	6.00
------	---	-------------	------

On X-Ray

653	"Medical Electricity" by Sinclair Tousey, M. D.....	<i>Extone</i>	10.00
1704	"Systematic Development of X-Ray Plates and Films" by Lehman Wendell, D. D. S.....	<i>Insure</i>	2.00
1707	"Roentgenotherapy" by Albert Franklin Tyler, M. D.....	<i>Indus</i>	2.75
1710	"U. S. Army X-Ray Manual." Prepared under the direction of the Division of Roentgenology and authorized by the Surgeon-General of the Army.....	<i>Infect</i>	5.00

On Actinic Ray Therapy

1744	"Actinic Ray Therapy" by T. Howard Plank, M. D.....	<i>Inlank</i>	5.00
1755	"Actinotherapy and Allied Physical Therapy" by T. Howard Plank, M. D.....	<i>Wagers</i>	7.50
1757	"Clinical Application of Sunlight and Artificial Radiation" by Edgar Mayer, M. D.....	<i>Wagone</i>	10.00
1977	"Basis of Light in Therapy" by Herman Goodman, M. D.....	<i>Wasted</i>	3.50

On the
Following pages
are Illustrated
Fischer
Complete Units
Including
Diathermy
X-Ray
Galvanic
Sine Wave
Radiant Therapy
and
Ultra-Violet Apparatus
also a
Price List of
Fischer
X-Ray Accessories
and Supplies

Price List of Fischer X-Ray Accessories and Supplies

No.	Description	Code	Price
1044	Aluminum Cassette, 8x10	Dermus	\$ 15.00
1045	Aluminum Cassette, 10x12	Derrid	17.00
1046	Aluminum Cassette, 11x14	Dew	19.00
1047	Aluminum Cassette, 14x17	Diad	21.00
385	Apron, Lead Protected	Amot	10.00
1626	Barium Sulphate, 1 lb. package	Barsul	.50
1066	Connector for Coolidge Tube	Baycon	1.00
409	Contactor for X-ray Timer	Fancon	85.00
1061	Controller for Coolidge Tube Filament	Cardin	30.00
447	Coolidge Tube Ammeter	Coamer	40.00
1060	Coolidge Filament Transformer	Cardia	50.00
1057	7-inch Fine Focus Coolidge Tube	Celery	125.00
1058	7-inch Medium Focus Coolidge Tube	Ccke	125.00
1059	7-inch Broad Focus Coolidge Tube	Cacal	125.00
1055	10 M. A. Coolidge Tube, Radiator Type	Celom	125.00
1056	30 M. A. Coolidge Tube, Radiator Type	Cedron	125.00
1054	Radiator Dental Coolidge X-ray Tube	Cella	125.00
1013	Coolidge Tube Shield for Radiator Type	Gaddo	35.00
1014	Coolidge Tube Shield, Dental Type	Gorget	35.00
523	Cord Reel, Single	Fagin	2.75
530	Cord Reel, Single, with Trolley Wheel	Hemoid	3.30
531	Cord Reel, Double, with Trolley Wheels	Hemp	7.50
525	Cord Reel Trolley Contacts	Hutt	.20
1601	Dark Room Safelight Ruby Lamp	Bath	1.75
1602	Dark Room Kodak Ruby Lamp	Bathco	3.50
1010	Dental Cone, Leaded Glass (short)	Carus	12.00
1011	Dental Cone, Leaded Glass (long)	Carlog	12.00
1182	Dental Film Clip, Single—dozen	Whilon	1.50
1183	Dental Film Holder, 10 clips—each	Whinny	1.75
1184	Dental Film Holder, 24 clips—each	Whiper	4.00
1646	Dental Film Holder—Fischer—dozen	Cascin	1.25
1632	Dental Film Holder—wooden—box of 10	Shapa	.25
1697	Dental Film Tank, glass	Impel	1.75
	Dental Film Mounts—Write for catalog		
1925	Developing Tank, Army Type	Unfit	81.00
1926	Developing Tank Cooling Arrangement	Ungot	6.00
1695	Developing Tank, 4-compartment	Ilium	72.50
1698	Developing Tank, Porcelain—2x9x14"	Image	7.00
1700	Developing Tank, Porcelain—2x15x20"	Impose	11.00
1701	Developing Tank, Porcelain—5x15x20"	Impugn	14.00
1604	Developing Tray, Steel Enameled—5x7"	Adeps	1.00
1605	Developing Tray, Steel Enameled—8x10"	Adler	1.75
1606	Developing Tray, Steel Enameled—10x12"	Agaric	2.25
1607	Developing Tray, Steel Enameled—11x14"	Agave	3.50
1608	Developing Tray, Steel Enameled—14x17"	Agnea	5.00
1715	Developing Frame for 5x7 Films	Incur	.75
1716	Developing Frame for 6½x8½ Films	Indeed	.85
1717	Developing Frame for 8x10 Films	Indent	1.25
1718	Developing Frame for 10x12 Films	Indry	1.50
1719	Developing Frame for 11x14 Films	India	1.75
1714	Developing Frame for 14x17 Films	Indict	2.00
555	Diagnostic Illuminator, 14x17"	Darest	16.50
551	Diagnostic Illuminator, 8x10"	Dartos	9.50
1080	Diaphragm, Bucky-Potter	Buckip	250.00
1007	Diaphragm, Lead, with 1" opening	Doom	.50
1008	Diaphragm, Lead, with 2" opening	Dory	.50
1650	Envelopes, Filing, 5x7—(100)	Fovea	1.15
1651	Envelopes, Filing, 6½x8½—(100)	Frax	1.30
1652	Envelopes, Filing, 8x10—(100)	Fret	1.50
1653	Envelopes, Filing, 10x12—(100)	Frost	2.00
1654	Envelopes, Filing, 11x14—(100)	Focus	2.50
1655	Envelopes, Filing, 14x17—(100)	Funda	3.50
1733	Exposure Rule, Eastman	Easex	2.50
1006	Filter, Aluminum—X-ray (1 mm.)	Donga	.25
683	Fixing and Hardening Powder (64 oz. size)	Braxy	.35
1020	Fluoroscope, Mounted, 5x7"	Drain	16.50
1021	Fluoroscope Screen, only, 5x7"	Drench	10.00
1022	Fluoroscope Screen, only, 8x10"	Duct	21.00
1023	Fluoroscope Screen, only, 10x12"	Dulcin	30.00
1017	Fluoroscope Screen, only, 11x14"	Dutch	40.00
1018	Fluoroscope Screen, only, 12x16"	Dyad	50.00
1019	Fluoroscope Screen, only, 14x17"	Dvne	60.00
1024	Fluoroscope, Mounted, Lead Glass Prot., 5x7"	Dulpro	20.00
1025	Fluoroscope, Mounted, Lead Glass Prot., 8x7"	Dull	21.50
1026	Fluoroscope, Mounted, Lead Glass Prot., 8x10"	Dulryo	40.00

Price List of Fischer X-Ray Accessories and Supplies


No.	Description	Code	Price
1027	Fluoroscope Screen, only—square inch	Dram	\$.25
1031	Fluoroscope, Patterson Operating Type	Patflu	45.00
1036	Fluoroscopic Screen and Frame, 10"x12"	Quaint	60.00
1037	Fluoroscopic Screen and Frame, 11"x14"	Quahn	65.00
1038	Fluoroscopic Screen and Frame, 12"x16"	Quantum	80.00
1039	Fluoroscopic Screen and Frame, 14"x17"	Quarry	100.00
380	Foil, X-ray Protection—(2½ lb. roll) lb.	Globe	.40
400	Foot Switch, X-ray	Fant	12.00
595	Glass Funnel—(8 oz. size)	Agria	.40
596	Glass Funnel—(16 oz. size)	Aque	.60
581	Glass Graduate—(8 oz. size)	Alalin	.40
582	Glass Graduate—(16 oz. size)	Alder	.60
201	Glass Stirring Rod	Advene	.15
361	Gloves, Leaded Rubber	Alsol	12.00
1012	Headrest, Chair Type	Calis	9.00
1040	Intensifying Screen, 8x10"	Diatom	10.00
1041	Intensifying Screen, 10x12"	Digest	15.00
1042	Intensifying Screen, 11x14"	Dinus	20.00
585	Kidney Compressor	Rubrum	2.50
573	Lead Lined Plate Chest	Dun	8.25
575	Lead Lined Plate Chest	Dens	15.00
577	Lead Lined Plate Chest	Deric	24.00
390	Leaded Glass—square inch	Glon	.08
1015	Leaded Glass Tube Shield	Gord	15.00
563	Lead Letters—for marking films	Forged	.05
1009	Lead Lined Cone—5½ inch diameter	Dura	5.00
1050	Lead Lined Cone—3 inch diameter	Buret	8.00
1051	Lead Lined Cone—8 inch diameter	Burn	8.00
1070	Lead Lined Treatment Cone—1 inch opening	Holz	5.00
1071	Lead Lined Treatment Cone—2 inch opening	Horn	5.00
1072	Lead Lined Treatment Cone—3 inch opening	Hovus	5.00
1073	Lead Lined Treatment Cone—4 inch opening	Huet	5.00
564	Lead Numbers—for identification	Forbid	.05
350	Lead Protection Screen	Alum	75.00
381	Lead Sheet—½ inch (pound)	Glonus	.20
570	Marker for X-Ray Films	Fames	5.50
445	Meter, X-Ray—0.15 M. A.	Extver	18.00
446	Meter, X-Ray—0.60 M. A.	Extobe	32.50
459	Meter, X-Ray—0.30 M. A.	Whistl	22.50
975	Plate Support	Dolor	17.50
1005	Tube Stand—X-Ray	Dossil	80.00
1648	X-ray Dental Films, slow	Bulla	1.50
1649	X-ray Dental Films, fast	Speed	1.50
1640	X-ray Dental Films, Eastman, fast	Brain	.70
1665	X-ray Dental Films, Eastman, slow	Bot	.15
680	X-ray Developer ½ gallon size	Laird	.85
681	X-ray Developer 1 gallon size	Lamboy	.20
1678	X-ray Exposure Holder, 5"x7"	Ladle	.30
1679	X-ray Exposure Holder, 6½"x8½"	Lagoon	.35
1680	X-ray Exposure Holder, 8"x10"	Ladder	.40
1681	X-ray Exposure Holder, 10"x12"	Laguna	.50
1682	X-ray Exposure Holder, 11"x14"	Labial	1.45
1683	X-ray Exposure Holder, 14"x17"	Cholin	2.30
1685	X-ray Duplitized Eastman Films, 5"x7"	Cronic	3.30
1686	X-ray Duplitized Eastman Films, 6½"x8½"	Chyle	5.20
1687	X-ray Duplitized Eastman Films, 8"x10"	Cina	6.60
1688	X-ray Duplitized Eastman Films, 10"x12"	Circle	10.05
1689	X-ray Duplitized Eastman Films, 11"x14"	Claret	1.45
1690	X-ray Duplitized Eastman Films, 14"x17"	Weaver	3.40
1985	X-Ray Films—Buck—5"x7"	Weevil	5.35
1986	X-Ray Films—Buck—8"x10"	Welkin	6.75
1987	X-Ray Films—Buck—10"x12"	Welter	10.30
1988	X-Ray Films—Buck—11"x14"	Whaler	1.75
1989	X-Ray Films—Buck—14"x17"	Wharve	4.10
1990	X-Ray Films—Buck—Non-inflam., 5"x7"	Wheale	6.40
1991	X-Ray Films—Buck—Non-inflam., 8"x10"	Wheel	8.15
1992	X-Ray Films—Buck—Non-inflam., 10"x12"	Wheeze	12.40
1993	X-Ray Films—Buck—Non-inflam., 11"x14"	Fanlie	48.00
1994	X-Ray Films—Buck—Non-inflam., 14"x17"	Echo	4.00
408	X-Ray Timer		
375	X-Ray Tube Rack—2 tube		
	X-Ray Tube repairs—write for prices.		
993	X-Ray Tube—6" Tungsten Target Transformer	Elbow	38.50
994	X-Ray Tube—7" Tungsten Target Transformer	Elder	43.50
997	X-Ray Tube—7" Tungsten Target H. F.	Elroid	43.50
998	X-Ray Tube—6" Tungsten Target H. F.	Elgon	58.50
1005	X-Ray Tube Stand	Possil	80.00

The Fischer Combination Electrophysiotherapeutic Treatment Outfit — Style "FO" Senior

A handsome, impressive piece of office equipment, compact, simple in operation yet the most powerful machine of its type available, and capable of the finest kind of results.

No.	Code	Price
1229	Apparatus as illustrated, with necessary connecting cords, Kolischer Spark Gap, Meter and Leyden Jars.....Nionly	\$685.00

Ask for pamphlet Form No. 430A.

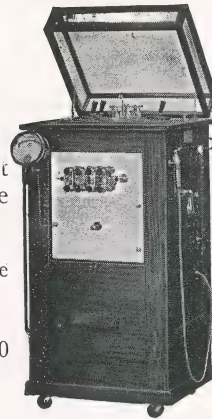


The Fischer Type "LO" Senior High Frequency Diathermy Apparatus

Designed especially for those physicians who are concerned with the specific application of medical and surgical diathermy (electro-coagulation), D'Arsonval auto-condensation and monopolar high frequency currents, but who have no desire for motor and pump features.

No.	Code	Price
1234	Apparatus as described, with necessary connecting cord, Kolischer Spark Gap, Meter and Leyden Jars.Nisenl	\$575.00

Ask for pamphlet Form No. 430A.

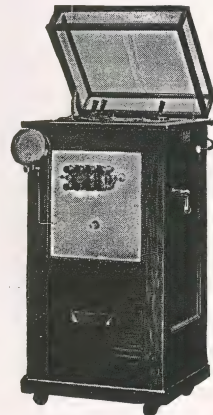

The Fischer Senior Model "V" Diathermy Apparatus


Embodies in one convenient cabinet every modality, at any voltage or milliamperage required in high frequency therapy. The "SENIOR" of the entire Fischer line of diathermy equipment.

No.	Code	Price
2100	Yacht	\$585.00

The Fischer Model "V" Senior Apparatus, with tissue-cutting current.

No.	Code	Price
2116	Yecut	\$685.00

Ask for descriptive pamphlet Form 1002A.

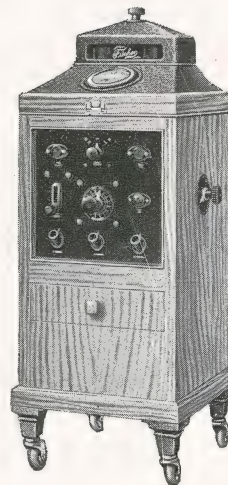

The Fischer Model "G-3" Diathermy Cabinet

"An Instrument of Precision,
Beautifully Mounted"

Efficient and Economical

No.	Code	Price
2125	Fischer Model "G-3" Diathermy Unit, with connecting cord and plug, but no accessories.....Ajax	\$385.00

Ask for pamphlet Form 1012A



The Fischer Portable Diathermy and Electrocoagulation Apparatus Type "GP2"

This unit is built into a black leatherette covered carrying case, with closed lid, making it in every sense a "portable" apparatus. While this is a very effective office machine, it is more adapted to bedside work.

No.	Code	Price
1393	With connecting cord, but no accessoriesVitat	\$285.00

Ask for descriptive pamphlet Form No. 869A





The Fischer Portable Diathermy and Electrocoagulation Apparatus, Type "G2"

No physician's office, no hospital or sanitarium is complete without some good physiotherapy equipment—particularly a diathermy apparatus of the portable or semi-portable type. Such a machine is a decided requisite if modern methods of medicine and surgery are to be employed. Apparatus and Cart sold separately.

No.	Code	Price
1390	With connecting cord, but no accessoriesVitic	\$305.00
1255	Walnut CartTerbo	40.00

Ask for descriptive folder Form No. 869A

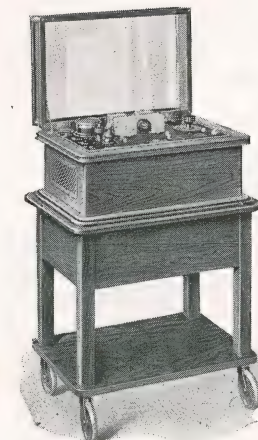

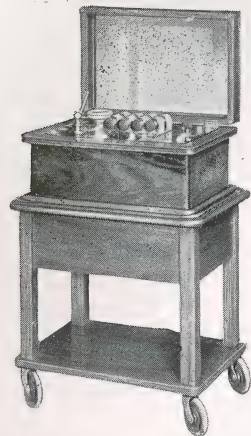

A Moderately Priced, Portable, High Frequency Diathermy Outfit, Model "A"

This equipment has been designed especially for use by physicians, hospitals and sanitariums where a convenient, efficient, portable machine of low price is required.

The Fischer Model "A" Diathermy Unit, in mahogany case with glass top, as illustrated, on mobile Hospital Cart No. 1255, with connecting cord and plug, but no accessories, for operation on 110 volt, 60 cycle alternating current.


No.	Code	Price
2042	Porcc	\$280.00

The Fischer Model "AP" Portable Diathermy Unit, in black carrying case, with connecting cord and plug, but no accessories, wound for operation on 110 volt, 60 cycle alternating current.

No.	Code	Price
2045	Poree	\$225.00



The Fischer Galvanic Current Generator

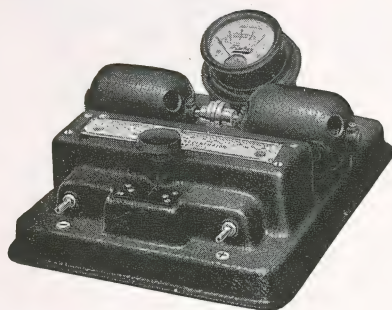

No.	Code	Price
1200	Complete with accessories...Galvan	\$125.00

The extreme importance of the galvanic current in the practice of modern medicine is recognized by the majority of physicians of today, in gynecology, urology, etc., for depilatory work, ionization, rectal lesions, electrolysis, strictures, etc., etc.

Ask for descriptive pamphlet Form No. 524A.

The Fischer Electro-Surgical Tissue Cutting Apparatus

Outfit is mounted in a black leatherette-covered carrying case. Weight only 49 pounds.

The very latest technic advocated by those surgeons who have made a study of electrical tissue cutting may be employed with this apparatus with an assurance of success.

No.	Code	Price
2130	Anco	\$225.00

Ask for descriptive pamphlet Form 1035



The Fischer Low Voltage Generator



A new and tremendously improved apparatus for the production of continuous or surging alternating or direct current. Currents available are: straight galvanism, surging galvanism, a direct current dwell wave, straight alternating at a very high frequency of oscillation, surging alternating, and an alternating dwell wave.

No.	Code	Price
2206	Complete with connecting cable and stand as illustrated	Appel \$495.00


Ask for descriptive pamphlet Form No. 1037

The Fischer Junior Portable Diathermy Apparatus

No. 2140. Fischer Junior Model "Y" Portable Diathermy Apparatus, with connecting cord and plug, ready to attach to the 110-volt, 60 cycle alternating current, with no accessories.

Code	Price
Wrathy	\$125.00

Ask for pamphlet Form No. 985A

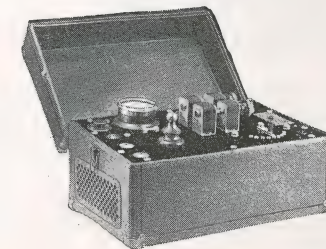


The Specialist's Eye, Ear, Nose and Throat Combination Cabinet

This new equipment is built in a lower cabinet than formerly, as most specialists sit down at this work and desire all the electrical outlets, atomizers, spray controls, etc., as near at hand as possible. These features have all been admirably taken care of on this apparatus.

No.	Code	Price
1203	Neuris	\$530.00


Ask for descriptive pamphlet Form No. 1007A.

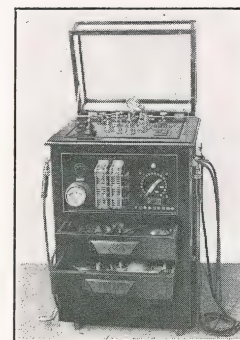

The Fischer Type "S" 30 Milliampere Coolidge Radiographic Unit

No.	Code	Price
1225		
Capacity, 30 M. A. at a 5-inch gap. Complete with connecting cords, accessories and supplies, including Coolidge Tube.....		
	Mater	\$850.00


Ask for pamphlet Form No. 353A.

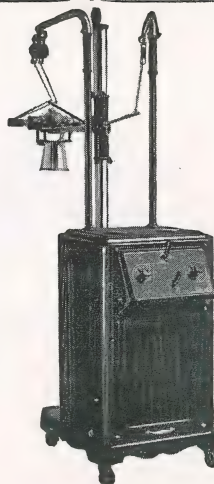

The Fischer Improved Interrupterless X-Ray Transformer Type "2-B"

No.	Code	Price
805		
Capacity, 60 M. A. at a 6-inch gap. With connecting cords and cord reels, only, no accessories (A. C.).....		
	Vacate	\$700.00

Write for pamphlet Form No. 341A.

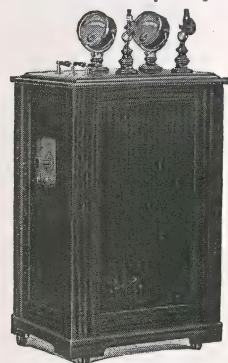


The Alpine Sun Lamp

No.	Code	Price
1400		
Mounted on Mobile Base		
	Meiny	\$440.00

Following our policy, this new model Alpine Sun Lamp is the outcome of observations and careful studies made of the use of the quartz lamps in the hands of the physicians. This apparatus is so constructed that it increases the efficiency of such work, making it more convenient to manipulate, and more durable.

Send for descriptive pamphlet

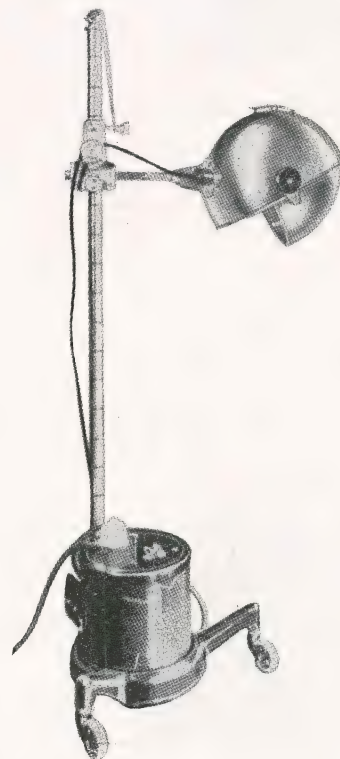


Prices on Hanovia Equipment are F. O. B. Newark, N. J.

Kromayer Lamp — Portable (Self-Contained Unit)

No.	Code	Price
1395		
	Wallet	\$615.00

Cooling system is contained within the standard, making outside water connections unnecessary. In the alternating current lamp the transformer is also contained in the standard. Self-suspending burner permits of free manipulation.

Send for descriptive pamphlet

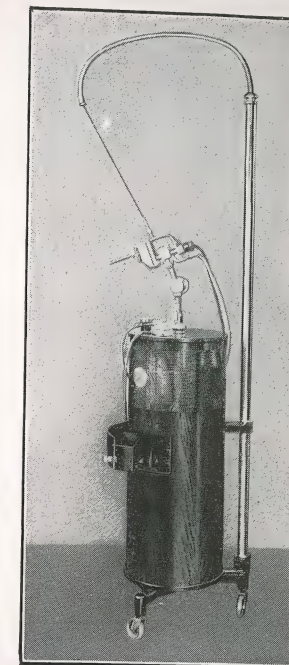


Combination Unit — Alpine Sun and Kromayer Lamps

No.	Code	Price
1422		
	Midst	\$795.00

By far the greatest effect of the sun's rays is due to the ultra-violet, but a more intense producer of ultra-violet rays is the quartz lamp. Here the rays are always available, always constant, and can be administered in quantity to give the desired results.

Both the Alpine Sun and Kromayer Lamps are producers of ultra-violet rays, that give the maximum intensity for therapeutic procedure.

Send for descriptive pamphlet

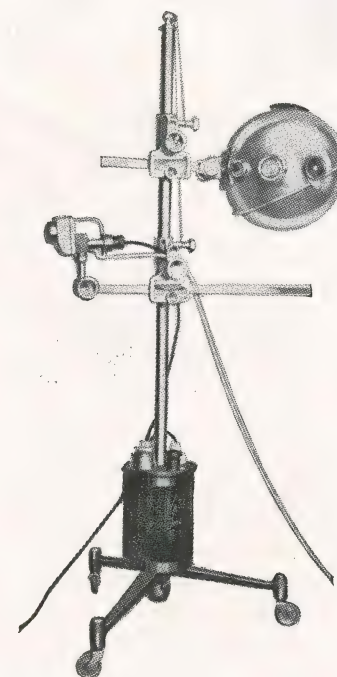


Prices on Hanovia Equipment are F. O. B. Newark, N. J.

The Kromayer Ultra-violet Lamp

No.	Code	Price
1418	Micro	\$495.00

This type presents a convenient and intense source of ultra-violet rays, with features and ability to function, far surpassing any other apparatus of similar purport.

Send for descriptive pamphlet

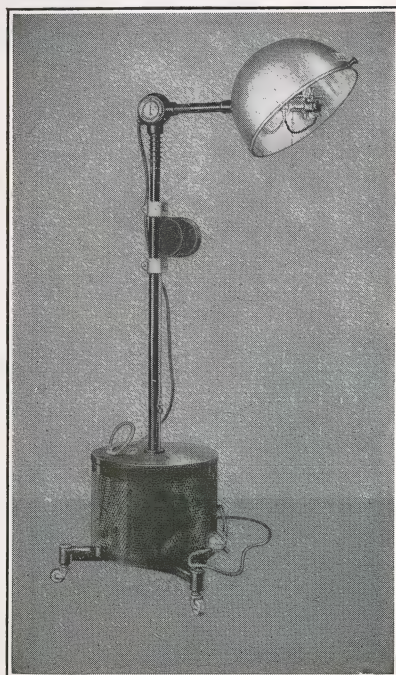

The "Luxor" Model Alpine Sun Lamp


The definite results accomplished through the use of quartz light therapy by the medical profession in treating disease, has made it patent that a quartz lamp be made for the patient's use in carrying out the treatments as prescribed by the patient's physician in his own home.

The Patient's Model Luxor Lamp is a very simple, compact, self-contained unit embracing many convenient devices and insuring flexibility in all usages, that may be prescribed for it, by the patient's physician.

No.	Code	Price
1397	Wigwag	\$300.00

Prices on Hanovia Equipment are F. O. B. Newark, N. J.

Reserve Burners for Hanovia Alpine and Kromayer Lamps Alpine Sun Lamp Burners

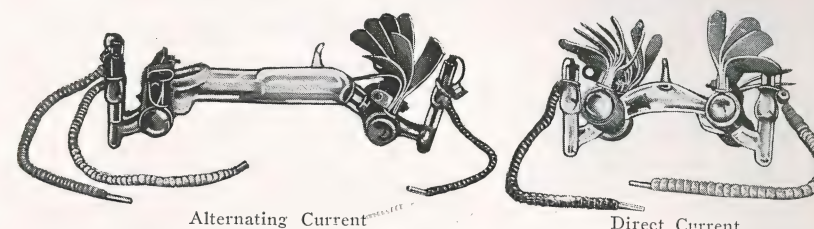


The Alpine Sun Lamp Burners have been regarded for many years as the most efficient type of quartz lamp burners manufactured. They are of the entire quartz mercury anode type.

Kromayer Burners

The Kromayer Burner is of the entire quartz mercury anode type. Its longer life and lower operating cost in comparison with other burners have been conclusively proved.

A service which is distinctive with HANOVIA is the repairing and exchanging of worn out or injured burners at a very nominal cost.

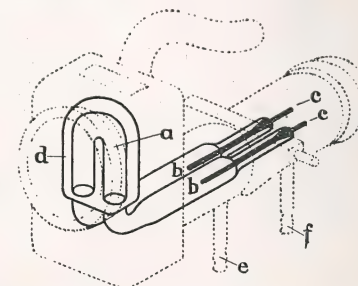

Price List

No.	Code	Price
750	Alpine Sun Lamp Burner (either 90-120 or 200-240 volt, 60 cycle alternating current).....	Wildly \$200.00
752	Kromayer Burner (either 90-120 or 200-240 volt, 60 cycle alternating current) in case, complete.....	Wimble 255.00
756	Alpine Sun Lamp Burner for direct current (90-120 or 200-240 volts)	Winery 128.00
758	Kromayer Burner for direct current (90-120 or 200-240 volts) in case, complete.....	Witily 175.00
(For other than 60 cycle, add \$50.00 to prices.)		

Hanovia Alpine and Kromayer Burner Repairs

These burners may be repaired or exchanged at the following prices:		
A. C. Alpine Burner Repair.....		\$60.00
D. C. Alpine Burner Repair.....		48.00
A. C. Kromayer Burner Repair.....		78.00
D. C. Kromayer Burner Repair		60.00
(These prices apply in all cases where all parts of the old burner are returned.)		
New metal cases for A. C. or D. C. Kromayer Burners.....		\$20.00

CARBON ARC LAMPS


We have a complete line of Carbon Arc Lamps, for ultra-violet, visible and infra-red radiation, ranging in price from \$48.50 to \$250.00.

The Fischer Twin Carbon Arc Lamp, Model "M," selling for only \$48.50 (see description on page 79).

An Automatic Single Arc Lamp for \$135.00. The National Twin Carbon Arc Lamp for \$137.50. The Duo-arc Automatic Twin Carbon Arc Lamp for \$250.00.

Details will be sent you on request.

Prices on Hanovia Equipment are F. O. B. Newark, N. J.

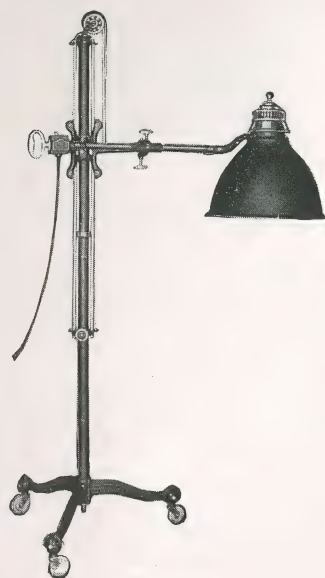


The Fischer "Superior" Radiant Therapy Lamp

No.	Code	Price
1295	Firaap	\$125.00

Medical literature abounds in reports of the desirability of light therapy in many conditions. There come to the mind of the progressive physician many instances where it is indicated as a curative, or a valuable adjunct and alleviative. The logic of light stands out pre-eminently.

Send for descriptive pamphlet
Form No. 674

Fischer "Superior" Radiant Therapy Lamp for Ceiling and Wall Suspension

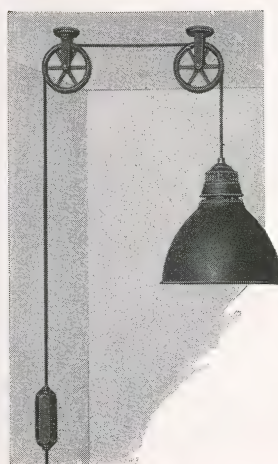


No.	Code	Price
1297..Wacker		\$82.50

At Left—Fischer "Superior" Radiant Therapy Lamp with Ceiling Suspension. Counterweight and Switch combined.

No.	Code	Price
1296..Wabble		\$110.00

At Right—Fischer "Superior" Radiant Therapy Lamp with Wall Bracket Suspension. Counterweight and Switch combined.

Send for descriptive
pamphlet No. 889

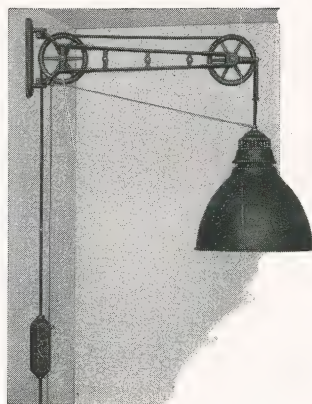


The New Fischer Twin Carbon Arc Lamp---

which delivers as much Ultra-violet, Visible and Infra-red Radiation as any Carbon Arc Lamp now on the market operating on a lighting circuit—and yet at a price of only \$48.50—with installments if you wish!


A new therapeutic lamp producing a spectrum of infra-red, visible and ultra-violet rays . . . epoch making in design, in efficiency and economy.

No.	Code	Price
2245	Twinal	\$48.50

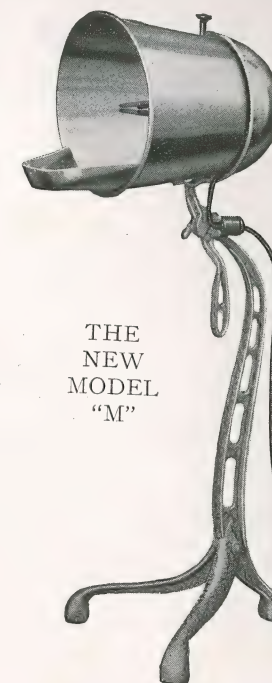

THE
NEW
MODEL
"M"

Informative Booklets on Diathermy

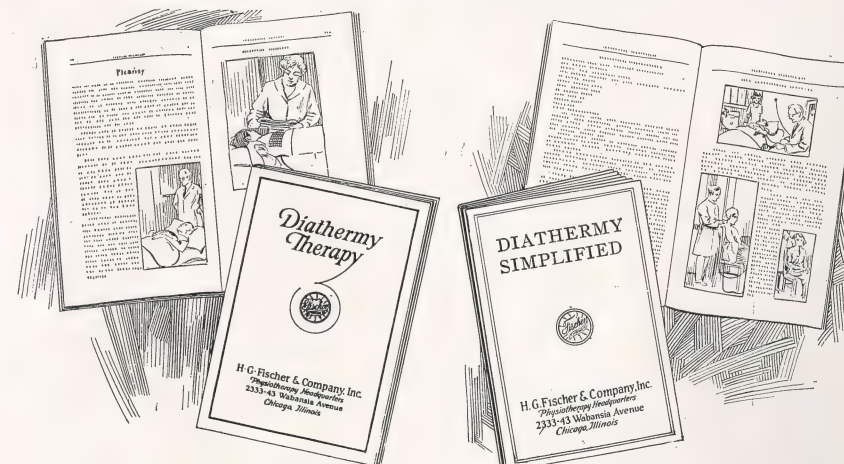

Diathermy Therapy

106 pages of standard technics, covering the various conditions in which Diathermy is indicated. Profusely illustrated. Price, \$1.00.

The Story of Diathermy

The history, theory and practice of this new branch of medical science. No charge.

Available Reprints on Various Physiotherapeutic Subjects

(Alphabetically by Author)

PLEASE NOTE: It is a pleasure to publish reprints for the good cause of better physical therapy, but it is quite an expensive procedure. We will appreciate it, therefore, if you will inclose stamps at the rate of 5 cents for each reprint desired. While this is a seemingly small matter, it will enable us to distribute more and better reprints on more varied subjects without effecting too great a hardship on ourselves.

Title	Form No.	Title	Form No.
Bau, H. W., M. D.—"Otitis Media, Zinc Ionization in".....	866	Elsom, J. C., M. D.—"Bell's Palsy, The Treatment of by Physiotherapy".....	810
Breuer, Miles J., M. D.—"Sciatica".....	658	Elsom, J. C., M. D.—"Physiotherapy in a State Hospital".....	907
Chapman, W. B., M. D.—"Hemorrhoids, Electro-Surgical Removal of".....	851	Ewerhardt, F. H., M. D.—"Joint Injuries, Diathermy in".....	708
Chapman, W. B., M. D.—"Surgical Diathermy".....	896	Ewerhardt, F. H., M. D.—"Orthopedic Surgery, Physiotherapy in".....	845
Chapman, W. B., M. D.—"The Uses of Physiotherapy"—"Diathermy in Gynecology".....	643	Fouts, R. W., M. D.—"Bone and Joint Injuries, Physiotherapy Treatment of".....	558
Chapman, W. B., M. D.—"Tuberculosis of the Cervical Lymph Glands".....	923	Giesy, J. U., M. D.—"Galvanism, A Discussion of".....	910
Chapman, W. B., M. D.—"Tuberculosis Treatment of by Physical Agents".....	711	Gradwohl, R. B. H., M. D.—"Physiotherapy Department in a Modern Hospital, Development of".....	857
Cherry, Thomas H., M. D.—"Pelvic Infections, Diathermy in".....	918	Granger Frank B., M. D.—"Physiotherapy in Low Back Conditions".....	844
Clark, Wm. L., M. D., Morgan, J. Douglas, M. D., and Asnis, Eugene J., M. D., "Neoplasms, The Treatment of, by Electrothermic Methods".....	920	Grant, Owsley, M. D.—"Gonorrheal Epididymitis, Diathermy in".....	949
Corbus, Budd C., M. D., and O'Connor, Vincent J., M. D.—"Diathermy—A Specific for Gonorrheal Epididymitis".....	530	Henry, E. C., M. D.—"Light in Infection".....	856
Corbus, Budd C., M. D., and O'Connor, Vincent J., M. D.—"The Treatment of Gonorrheal Endocervicitis by Heat".....	571	Henry, E. C., M. D.—"Physiotherapy as Used by the General Surgeon".....	882
Crile, G. W., M. D.—"Conserving the Temperature of the Viscera Before and After Abdominal Operations, by Diathermy".....	900	Hollender, A. R., M. D., and Cottle, M. H., M. D.—"Hypocalcemia in Hay Fever and Asthma".....	855
Cumberbatch, Elkin P., Dr.—"Discussion on Diathermy".....	1011	Hollender, A. R., M. D., and Cottle, M. H., M. D.—"Nasal Accessory Sinus Disease, Treatment of".....	912
Cumberbatch, Elkin P., Dr.—"Gonococcal Infections, Treatment of by Diathermy".....	903	Hollender, A. R., M. D., and Cottle, M. H., M. D.—"Physical Agents in Partial Deafness".....	913
Deutsch, William F., M. D.—"Electrocoagulation of Hemorrhoids".....	1016	Hollender, A. R., M. D., and Cottle, M. H., M. D.—"Radiant Energy in the Treatment of Otitis Media".....	853
Dillinger, G. A., M. D.—"Technic of Tonsil Electrocoagulation (Diathermy) With report of one hundred and fifty cases".....	1018	Kobak, Disraeli, M. D.—"Physiotherapy in Surgical and Post-Surgical Conditions".....	843
Duval, Emile C., M. D.—"Physiotherapy, The Economic Value of".....	905	Kolischer, Gustav, M. D.—"Diathermy to the Heart".....	663
Duval, Emile C., M. D.—"The Application of Diathermy and Its Technic".....	902	Kolischer, Gustav, M. D.—"Medical Kidney Diseases, Diathermy in".....	90
		Kolscher, Gustav, M. D.—"The Uses of Physiotherapy"—"Principles of Surgical Diathermy".....	646

Title	Form No.	Title	Form No.
McFee, William D., M. D.—"Electrocoagulation in Surgery".....	849	Pope, Curran, M. D.—"Tuberculosis, the Role of Physical Agents in the Treatment of".....	926
Milligan, Sir William, M. D.—"Radio-Diathermy in Inoperable Diseases of the Air Passages".....	978	Pope, Curran, M. D.—"When Shall We Treat the Painful Point".....	895
Morse, F. H., M. D.—"Galvanism, a Plea for".....	639	Pope, Curran, M. D.—"White or Blue Globes for Radiant Therapy".....	819
Morse, F. H., M. D.—"Measured Wave Currents".....	528	Rowell, Carlton L., M. D.—"The Uses of Physiotherapy"—"Chronic Gonorrhea and Its Complications".....	657
Otis, Lloyd M., M. D.—"Gastro-Intestinal Stasis, Sinusoidal Currents in".....	911	Stewart, Harry Eaton, M. D.—"Diathermy in Pneumonia, a Report of Ten Cases".....	489
Otis, Lloyd M., M. D.—"Industrial Surgery, Physiotherapy in".....	919	Stewart, Charles E., M. D.—"Galvanism".....	898
Otis, Lloyd M., M. D.—"Physiotherapy in Relation to Surgical Conditions".....	977	Tyler, Albert F., M. D.—"The Uses of Physiotherapy"—"Surgical Diathermy in Benign Skin Blemishes".....	645
Pettit, Roswell T., M. D.—"Heliotherapy".....	854	Van Putte, P. J., M. D.—"Gonorrhea in Women, Diathermy of Thermopenetration in the Treatment of".....	947
Pope, Curran, M. D.—"Gastric and Duodenal Ulcer, The Physiotherapeutic Treatment of".....	893	Walke, Frank H., M. D.—"Gynecological Conditions, Electrophysiotherapy in the Treatment of".....	948
Pope, Curran, M. D.—"Post Influenzal State, Management of".....	917	Waring, J. B. H., M. D.—"Electrocoagulation of Hemorrhoids".....	883
Pope, Curran, M. D.—"Prostatitis".....	894	Wyeth, George M., M. D.—"A Further Study of Endothermy in Accessible Malignancy".....	850
Pope, Curran, M. D.—"The Uses of Physiotherapy"—"Renal Diseases".....	644		

(Alphabetically by Subjects)

Title	Form No.	Title	Form No.
Application of Diathermy.....	902	Electrocoagulation of Hemorrhoids.....	883
By Emile C. Duval, M. D.		By J. B. Waring, M. D.	
Bell's Palsy, The Treatment of, by Physiotherapy.....	810	Endothermy in Accessible Malignancy.....	850
By J. C. Elsom, M. D.		By George M. Wyeth, M. D.	
Bone and Joint Injuries, Physiotherapy Treatment of.....	558	Galvanism.....	898
By R. W. Fouts, M. D.		By Chas. E. Stewart, M. D.	
Conserving the Temperature of the Viscera Before and After Abdominal Operations, by Diathermy.....	900	Galvanism, A Discussion of.....	910
By G. W. Crile, M. D.		By J. U. Giesy, M. D.	
Deafness, Partial—Physical Agents in.....	913	Galvanism, A Plea for.....	639
By A. R. Hollender, M. D., and M. H. Cottle, M. D.		By F. H. Morse, M. D.	
Diathermy, Discussion on.....	1011	Gastric and Duodenal Ulcer, The Physiotherapeutic Treatment of.....	893
By Dr. Elkin P. Cumberbatch.		By Curran Pope, M. D.	
Diathermy to the Heart.....	663	Gastro-Intestinal Stasis, Sinusoidal Currents in.....	911
By Gustav Kolischer, M. D.		By Lloyd M. Otis, M. D.	
Electrocoagulation in Surgery.....	849	Gonococcal Infections, Treatment of, by Diathermy.....	903
By Wm. D. McFee, M. D.		By Elkin P. Cumberbatch, Dr.	

Title	Form No.
Gonorrhea, Chronic, and Its Complications.....	657
By Carlton L. Rowell, M. D.	
Gonorrhea in Women, Diathermy or Thermopenetration, in the Treatment of.....	947
By P. J. Van Putte, M. D.	
Gonorrheal Endocervicitis, The Treatment of—by Heat.....	571
By Budd C. Corbus, M. D., and Vincent J. O'Connor, M. D.	
Gonorrheal Epididymitis, A Specific for.....	530
By Budd C. Corbus, M. D., and Vincent J. O'Connor, M. D.	
Gonorrheal Epididymitis, Diathermy in.....	949
By Owsley Grant, M. D.	
Gynecological Conditions, Physiotherapy in the Treatment of.....	948
By Frank H. Walke, M. D.	
Gynecology, Diathermy in.....	643
By W. B. Chapman, M. D.	
Heliotherapy.....	854
By Roswell T. Pettit, M. D.	
Hemorrhoids, Electrocoagulation of.....	1016
By William F. Deutsch, M. D.	
Hemorrhoids, Electro-surgical Removal of.....	851
By W. B. Chapman, M. D.	
Hemorrhoids, Electrocoagulation of.....	883
By J. B. H. Waring, M. D.	
Hypocalcemia in Hay Fever and Asthma.....	855
By A. R. Hollender, M. D., and M. H. Cottle, M. D.	
Industrial Surgery, Physiotherapy in.....	919
By Lloyd M. Otis, M. D.	
Joint Injuries, Diathermy in.....	708
By F. H. Ewerhardt, M. D.	
Kidney Diseases, Medical—Diathermy in.....	908
By Gustav Kolischer, M. D.	
Light in Infection.....	856
By E. C. Henry, M. D.	
Nasal Accessory Sinus Disease, Treatment of.....	912
By A. R. Hollender, M. D., and M. H. Cottle, M. D.	
Neoplasms, The Treatment of, by Electrothermic Methods.....	920
By Wm. L. Clark, M. D., J. Douglas Morgan, M. D., and Eugene J. Asnis, M. D.	
Orthopedic Surgery.....	845
By F. H. Ewerhardt, M. D.	
Otitis Media, Radiant Energy in the Treatment of.....	853
By A. R. Hollender, M. D., and M. H. Cottle, M. D.	
Otitis Media, Zinc Ionization in.....	866
By H. W. Bau, M. D.	
Pelvic Infections, Diathermy in.....	918
By Thomas H. Cherry, M. D.	
Physiotherapy as Used by the General Surgeon.....	882
By E. C. Henry, M. D.	
Physiotherapy Department in a Modern Hospital, Development of.....	857
By R. B. H. Gradwohl, M. D.	

Title	Form No.
Physiotherapy in a State Hospital.....	907
By J. C. Elsom, M. D.	
Physiotherapy in Low Back Conditions.....	844
By Frank M. Granger, M. D.	
Physiotherapy in Relation to Surgical Conditions.....	877
By Lloyd M. Otis, M. D.	
Physiotherapy, The Economic Value of.....	905
By Emile C. Duval, M. D.	
Physiotherapy, The Uses of.....	643
By W. B. Chapman, M. D.	
Physiotherapy, The Uses of.....	646
By Gustav Kolischer, M. D.	
Physiotherapy, The Uses of.....	644
By Curran Pope, M. D.	
Pneumonia, Diathermy in, A Report of Ten Cases.....	489
By Harry Eaton Stewart, M. D.	
Post-Influenzal State, The Management of.....	917
By Curran Pope, M. D.	
Prostatitis.....	894
By Curran Pope, M. D.	
Radiant Therapy, White or Blue Globes.....	819
By Curran Pope, M. D.	
Radio-Diathermy in Inoperable Diseases of the Air Passages.....	978
By Sir Wm. Milligan, M. D.	
Renal Diseases.....	644
By Curran Pope, M. D.	
Sciatica.....	658
By Miles J. Breuer, M. D.	
Surgical and Post-Surgical Conditions, Physiotherapy in.....	843
By Disraeli Kobak, M. D.	
Surgical Diathermy.....	896
By W. B. Chapman, M. D.	
Surgical Diathermy in Benign Skin Blemishes.....	645
By Albert F. Tyler, M. D.	
Surgical Diathermy, The Principles of.....	646
By Gustav Kolischer, M. D.	
The Uses of Physiotherapy.....	657
By Carlton L. Rowell, M. D.	
Tonsil Electrocoagulation (Diathermy), Technic of—With report of one hundred and fifty cases.....	1018
By G. A. Dillinger, M. D.	
Tuberculosis of the Cervical Lymph Glands.....	923
By W. B. Chapman, M. D.	
Tuberculosis, The Role of Physiotherapy Agents in the Treatment of.....	926
By Curran Pope, M. D.	
Tuberculosis, The Treatment of—by Physical Agents.....	711
By W. B. Chapman, M. D.	
Uses of Physiotherapy.....	645
By Albert F. Tyler, M. D.	
Wave Currents, Measured.....	528
By F. H. Morse, M. D.	
When Shall We Treat the Painful Point?.....	895
By Curran Pope, M. D.	

H. G. FISCHER & Co., INC.

ORDER FORM

In ordering please be sure to specify names and catalogue numbers of articles wanted, also sizes, etc., and use code number if order is telegraphed.

Ordered by _____

Address _____

City _____ State _____

(In placing first order it is generally best to send cash with order or have goods come C. O. D.)

Also send the following literature:

INDEX

A

Adapters, Cord Tip.....	45
Adjustable High Frequency Handle	41
Adjustable Reaction Electrode.....	16
Air Hammer Vibrator.....	57
Air Heater	62
Alpine Sun Lamp Accessories.....	54-55
Applicators, Quartz	54-55
Applicators, Vibratory	59
Arc Carbons	53
Atomers	61
Autocondensation Cushions	17
Autocondensation Handles	17
Autocondensation Pad	18

B

Bags, Sand	9
Bandage, Elastic	10
Bath Speculum Wire.....	20
Baumanometer	33
Belt Electrode	25
Belt Mesh Electrode.....	21
Biaural Cords	32
Bierman Hemorrhoid Clamp.....	20
Binder, Lurie	10
Bladder Fulguration Electrode.....	43
Block Tin	11
Blower, Powder	61
Books	66
Bottles, DeVilbiss	61
Bottle, Suction	62-65
Breuer Safety Switch.....	30
Bulbs for Therapeutic Lamps.....	53
Burners, Infra Red.....	52

C

Carbon Ball Electrode.....	23-26
Carbon Hemorrhoid Electrodes.....	28
Carbons, Therapeutic Arc.....	53
Casters	56
Cataphoric Electrode	24
Cautery Cords	46
Cautery Handle	49
Cautery Knives	48-49
Cautery Transformer	47
Cavity Vibratodes	58
Chair Pad, Autocondensation.....	18
Chapman Vaginal Electrode.....	19
Clamp, Diathermy	8-11-30
Clamp Electrode, Diathermy.....	8-30
Condenser, Leyden Jar.....	35

Condensers, Static Arrester.....	56
Cone, Pennington	58
Connecting Wires	29
Connector for DeVilbiss Bottles.....	60
Connector for Liquid Bath.....	10
Connector for Rubber Cups.....	65
Contact Holder	11
Copper Ball Electrodes.....	23-26-27
Corbus Auto Pad.....	17
Corbus Endocervicitis Electrode.....	21
Cord Connector, Multiple.....	8
Cords, Cautery	46
Cords, Diathermy	12
Cords, High Frequency.....	42
Cords, Sinusoidal	29
Connector for Mesh Electrodes	8-11
Converters, Rotary	50-51
Cuffs, Mesh	7
Cups, Glass Exhaust.....	64
Cups, Rubber Exhaust.....	65
Cushion, Auto-Condensation	17
Cut-off, Special DeVilbiss.....	62

D

DeVilbiss Bottles	61
DeVilbiss Connector	60
Diagnostic Illuminator	45-46
Diagnostic Lamp Bulb.....	45-46
Diagnostic Transformer	47
Diathermy Belt Electrode.....	25
Diathermy Binder	10
Diathermy Clamp	8-30
Diathermy Clamp Electrode.....	8-30
Diathermy Hand Electrodes.....	13
Diathermy Paste	9
Diathermy Thermometer	20
Dilators, Pope	57
Dillinger Electrocoagulation Electrode	15
Disc Diathermy Electrodes.....	12
Disc, Spongio	29
Doane Turbinate Electrodes.....	16

E

Ear Electrode, Linn.....	32
Ear Electrode, Vacuum.....	43
Ear Speculum	31
Ear Vibratode	59
Elastic Bandage	10
Electrode, Adjustable Reaction.....	16

Electrode Clips	11	Handle, Shock Proof.....	39
Electrodes, Flexible Pad.....	13	Handle, Tissue Cutting.....	15
Electrodes, Fulguration	42-43	Handles, d'Arsonval	17
Electrode, Funck	22	Handles, High Frequency	37-39-44
Electrodes, High Frequency.....	36 to 40	Handles, Sinusoidal	30
Electrodes, Internal	27	Handles, Treatment	30-44
Electrodes, Mesh	6-7	Hawkeye Timer	30
Electrodes, Sponge	7	Headband and Electrodes.....	31
Electrodes, Prostatic	21-23-26-27	Heater, Air	62
Electrode Support, Morse.....	27	Heavy Cautery Handle.....	49
Electrode, Tonsil, Thometz.....	16	Heavy Cautery Knives.....	48-49
Electrodes, Disc	12	Hemorrhoid Clamp	20
Electrodes, Hand	13	Hemorrhoid Electrodes, Carbon	28
Electrodes, Surgical	14-15	High Frequency Cords.....	42
Electrodes, Urethral	18-22	High Frequency Cushion (Auto-Condensation)	17-18
Electrodes, Vacuum	36 to 40	High Frequency Electrodes, Non-Vacuum	40
Electrolytic Salt	35	High Frequency Electrodes	36 to 40
Endocervicitis Electrode, Chapman	19	High Frequency Handles.....	37-39-41-44
Endocervicitis Electrode, Corbus.....	21	High Frequency Meters	34
Epididymis Electrode	16	Holder for Galvanic Needles.....	29
Eustachian Tube Opener.....	61	Hollender-Cottle Headband	31
Exhaust Filter	63	Hollender-Cottle Nasal Speculum.....	54
Eye Cup, Galvanic.....	23		
Eye Magnet	45		
F		I	
Filter for Exhaust.....	63	Infra-red Burners	52
Finger Rheostat, Fulguration Device	13	Infra-red Lamps	52
Fischer-Morse Adapter	28	Indirect Treatment Handle.....	44
Flexible Sigmoid Electrode.....	24	Insulated High Frequency Electrodes	38-39
Foot Switch, Electro-coagulation.....	16	Insulated High Frequency Handles	39-41
Fulguration Electrodes	42-43	Internal Metal Electrodes.....	20 to 27
Fulguration Electrode, Bladder.....	43	Interrupter Handle	24
Fulguration Wire	42	Interrupter Points, Tungsten.....	35
Funck Penile Electrode.....	22	Intra-uterine Electrodes	22
Fuse, Meter Protection.....	34		
G		K	
Galvanic Needle Holder.....	29	Knives for Tissue Cutting.....	15
Galvanic Needles	29	Knives, Cautery	48-49
Galvanic Eye Cup	23	Knotts' Surgical Electrode.....	15
G. U. Auto Pad	17	Kolischer Parametric Electrode.....	20
Generator, Ozone	44	Kolischer Spark Gap	33
Glass Specula	20	Kromayer Lamp Accessories.....	54-55
Glass Vacuum Cups.....	64		
Glass Vacuum Handle	44		
Grease for Motor and Pump.....	65		
H		L	
Hand Diathermy Electrode	13	Lamp, Pilot	56
Handle, Cautery	49	Lamps, Infra-red	52
Handle, Interrupter	24	Lamps, Therapeutic	53
		Leyden Jars	35
		Linn Ear Electrode and Control.....	32

Liquid Bath Connector.....	10	Q	
Lurie Binder	10	Quartz Applicators	54-55
		Quartz Mercury Electrodes.....	41
M		R	
Magnet, Eye	45	Radiolites	53
Mansur Prostatic Electrode.....	21	Rectal Cone (Pennington).....	58
Mercury Quartz H. F. Electrodes	41	Rectal Electrode, Flexible.....	26-27
Mesh Belt Electrode.....	21	Rectal Electrode, Two Pole.....	24
Mesh Electrode Connector	8-11	Rectal Specula, Glass.....	20
Mesh Electrodes	6-7	Retractor, Pillar	15
Mesh Sponge Electrodes.....	7-8	Rotary Converters	50-51
Mesh Cuffs	7	Rowell Urethral Electrode Set.....	18
Milliampere Meters	34	Rubber Vacuum Cups.....	65
Moist Pad Electrodes.....	25		
Morse Electrode Support.....	27	S	
Morse-Fischer Adapter	28	Salt, Electrolytic	35
Motor Grease	65	Sandbags	9
Multiple Section Spark Gap.....	33	Shield for Diagnostic Lamp.....	45
Muscle Testing Pads.....	28	Sigmoid Electrode	23-27
		Sigmoid Electrode, Flexible.....	24
N		Sinusoidal Cords	29
Nagelschmidt Condensation Electrodes	41	Sinusoidal Handles	30
Nasal Speculum	54	Sinus Suction Bottle, Fischer.....	65
Nebulizer	61	Sinus Suction Tube.....	60
Needle Holder, Galvanic.....	29	Sound Vibratode	59
Needles, Galvanic	29	Spark Gap, Kolischer.....	33
Non-vacuum High Frequency Electrodes	40	Spark Interrupter Points, Tungsten	35
		Specula, Glass	20
O		Speculum, Ear	31
Oil for Refilling Transformers.....	34	Speculum, Nasal	54
Ozone Generator	44	Speculum, Wire Bath.....	20
		Sponge Mesh Electrode.....	7
P		Spongio Disc	29
Pad Electrodes	13-25	Starting Boxes for Rotary Converter	51
Pads for Autocondensation.....	17-18	Static Arrester (Condenser).....	56
Parametric Electrode	20	Suction Bottles	62-65
Paste, Diathermy	9	Suction Tube for Sinus.....	60
Penile Electrode, Funck	22	Support for Morse Electrodes.....	27
Pennington Rectal Cone.....	58	Surgical Diathermy Electrodes.....	14-15
Pilot Lamp	56	Switch, Foot, Electro-coagulation.....	16
Pillar Retractor	15	Switch, Safety	30
Plank Surgical Diathermy Electrode	15		
Pneumatic Vibratodes	57-58-59	T	
Pope's Dilators	57	Table, Treatment	18
Powder Blower	61	Testing Pads, Small Muscle.....	28
Pressure Handle	60	Therapeutic Arc Carbons.....	53
Pressure Tubing	60	Therapeutic Lamps	53
Pressure Valve Attachment	63	Thermometer, Diathermy	18-20
Prostatic Electrode	21-23-27	Thometz Tonsil Electrodes.....	16
Pump Grease	65	Timers Treatment	30

H. G. FISCHER & COMPANY, Inc.

Tin for Diathermy Electrodes.....	11	Urethral Sounds	22
Tissue Cutting Handle and Knives	15		
Tissue Cutting Apparatus.....	72	V	
Tongue Depressor	46	Vaginal Electrode, Metal.....	
Tonsil Electrode, Plank.....	15		19-21-23-24-27
Tonsil Electrode, Thometz.....	16	Vaginal Electrode, Two Pole.....	24
Tonsil Electrode, Knotts.....	15	Vaginal Specula, Glass.....	20
Transformer, Cautery and Diag- nostic	47	Valve Attachment, Pressure.....	63
Transformer Oil	34	Valve Cut-off, DeVilbiss.....	62
Treatment Table	18	Valve, Vacuum	63
Tubing, Pressure	60	Vibratodes	58-59
Tungsten Lamp (Diagnostic).....	45-46	Vibratodes for Air Hammer.....	57
Tungsten Spark Points	35	Vibratodes, Pneumatic	58-59
Turbinate Electrodes	16	Vibrator, Air Hammer.....	57
		Volt Control	32
U			
Ultra-violet Accessories	54-55	W	
Universal Diathermy Clamp.....	8	Wire Bath Speculum.....	20
Urethral Electrodes	18-22	Wire, Fulguration	42

Fischer Accessories



H·G·Fischer & Company, Inc.
Physical Therapy Headquarters
2323-37 Wabansia Avenue
Chicago, Illinois